EURUS S8 INSTRUCTIONS FOR USE

Dear Customers

Dear Customers

Thank you for purchasing our product.

This booklet explains how to use EURUS.

Before using EURUS, carefully read the operating instructions and make sure to use the product correctly.

Using the product without reading these instructions may lead to an accident.

For easy access to the information contained herein, keep this booklet at hand and review it as needed.

Ask your local authorized Belmont dealer to install this product by following the installation instructions contained in the product.

If you have any questions regarding the operating instructions or this product, contact your local authorized Belmont dealer.

If you find any dirt on or damage to the booklet and need a new booklet, report the catalog number indicated below to your local authorized Belmont dealer to order a new one.

This document describes the full version of the system. It may therefore cover components that are not included in the system you purchased.

2025-09-01	(6th edition)
REF	1E09WLF0

	Dea	r Custo	mers	2
1	Ge	neral I	nformation	
	1–1	Intende	d Purpose of the Product	8
	1–2	Complia	ance with Regulation and Directive	3
	1–3	Declara	tion of Conformity	3
	1–4	How to	Dispose of the Device	
	1–5		al of Residues	
	1–6	•	e to the user and/or patient	
	1–7		tible Handpieces	
	1–8		tible Dental Lights	
	1–9		S	
	1–10	_	al Description	
2	Sat	fety Co	onsideration	
	2–1	Risk Lev	vel Interpretation	16
	2–2		Precautions	
		•	to remember when operating the product	
	2–3		ns Where Caution Labels Are Attached	
	2–4	EMC Int	formation	34
	2–5	Compat	tible Handpieces	38
	2–6	Compat	tible Dental Lights	38
3	Pre	ecautic	ons for Use	
	3–1	Operatir	ng Precautions	39
	3–2		tions for Using Synthetic Leathers	
4	Pro	duct S	Specifications	
	4–1	Technic	al Data	42
		4-1-1	Specification Variations	42
		4-1-2	S8	
		4-1-3	Specifications for Air/Water/Suction	50
	4–2	System	Overview	51
	4–3	Name o	of Each Part	54
		4-3-1	Chair	54
		4-3-2	Headrest	
		4-3-3	Foot Controller (wired/wireless)	56

		4–3–4 Foot Switch	56
		4–3–5 Doctor Unit	57
		4-3-6 Cuspidor Unit	59
		4-3-7 Vac Pac Unit	61
		4–3–8 Assistant Unit	61
		4–3–9 Junction Unit	61
5	Оре	eration	
	5–1	Preparation Before Use	62
	5–2	After use	66
	5–3	Operating the main switch for chair during treatment (when the main switch for chair is available)	67
	5–4	Raising/lowering the chair and raising/reclining the backrest (manual operation)	
	5–5	Moving the chair to the preset position (automatic operation)	
	5–6	Operating the headrest (manual type)	
	5–7	Operating the headrest (electrohydraulic type)	
	5–8	Turning the armrest	
	5–9	Operating the doctor table	
	5–10	Control of the assistant tray	
	5–11	Handpiece	
		Doctor's unit operation panel	
		Assistant operation panel	
		Cancellation function	
		Lock function	
		5-15-1 Chair lock function	
		5–15–2 Handpiece lock function	
	5–16	Micromotor	
		Setting the micromotor slide mode (NBX/NLX plus/NLX nano/MX2/MCX)	116
		Setting the maximum rotation (NBX/NLX plus/NLX nano/MX2/MCX)	
		Memory setting for starting condition after powering on (NBX/NLX plus/NLX nano/MX2/MCX)	
		Gear conversion display function (NBX/NLX plus/NLX nano/MX2/MCX)	119
		Overheating prevention function (NBX/NLX plus/MX2/MCX)	120
		NLX plus	121
		MX2	123
	5–17	Ultrasonic scaler	130
		Perio/Endo/Scaling switch setting	130
		Setting of the maximum output in the slide mode Va	131
		Setting of the maximum output in the slide mode Fix	131

		Memory setting for starting condition after powering on	132
	5–18	3 Air turbine/motor	133
		Setting of the slide mode	133
		Setting of the maximum output	134
		Memory setting for starting condition after powering on	135
	5–19) Implant motor	136
		5-19-1 Connection method	136
		5-19-2 Operation method	140
		5-19-3 Setting handpiece conditions	141
		Setting the slide mode	141
		Setting the maximum output	141
		Setting default power-on memories	143
		Gear conversion display function (MX-i LED 3rd Gen.)	144
	5–20) Syringes	145
	5–21	Foot controller (wired/wireless)	146
		5-21-1 Confirmation of the pairing of the wireless foot controller	147
		5-21-2 How to replace batteries of the wireless foot controller	148
		5-21-3 Cable connection of a wireless foot controller	149
		5–21–4 Operating precautions for the wireless foot controller	
	5–22	2 Maintenance panel	151
	5–23	3 Handpiece (assistant holder)	152
	5–24	Assistant hose clamp	152
	5–25	5 Filling a Cup	153
	5–26	S LED indicator	154
	5–27	Water bottle	155
	5–28	3 USB port	156
	5–29	EURUS Light	157
	5–30) 900 Dental Light	158
	5–31	Monitor bracket	159
	5–32	2 Panoramic viewer	159
	5–33	B Dental viewer	
		Right/Left handed dentistry conversion	
	0 0 .		
6	Set	tting/Adjustment	
	6–1	Setting for automatic operation	168
		6-1-1 Setting the treatment and entry/exit positions	168
		6-1-2 Setting the mouth rinsing position	168
	6–2	Function switch	169

	6-2-1	Setting items with the function switch	
	6-2-2	Selecting the flushing method and carrying out flushing	17
	6-2-3	Selecting the vacuum line washing method and conducting washing	19
	6-2-4	Displaying the drive air pressure	208
	6-2-5	Setting the spray mode	209
	6-2-6	Setting the light activation timing	210
	6-2-7	Setting the micromotor brightness	21
	6-2-8	Setting the cupfiller water level	213
	6-2-9	Setting the cup-filling/bowl flush interlock	215
	6-2-10	Setting the bowl flush time	216
	6-2-11	Setting the language	217
	6-2-12	Setting the timer alarm tone	218
	6-2-13	Setting the key touch volume	219
	6-2-14	Setting the sleep mode time	220
	6-2-15	Setting emergency cancellation of the chair lock	22
	6-2-16	Displaying the program version	222
6–3	Adjusting	g the quantity of water/air supplied from the doctor unit	223
6–4	Adjustin	g the quantity of water/air supplied to the cuspidor unit	224
Ma 7–1		nce and Cleaning	22
	Exterior.		
7–1	Exterior.	Cleaning and disinfecting the surfaces	225
7–1	Exterior. 7-1-1 Chair	Cleaning and disinfecting the surfaces	225
7–1 7–2	Exterior. 7–1–1 Chair 7–2–1	Cleaning and disinfecting the surfaces	225 226
7–1 7–2	Exterior. 7-1-1 Chair 7-2-1 Doctor u	Cleaning and disinfecting the surfaces Leather part unit	225 226 226
7–1 7–2	Exterior. 7–1–1 Chair 7–2–1	Cleaning and disinfecting the surfaces Leather part unit Touch panel	226 226 227
7–1 7–2	Exterior. 7-1-1 Chair 7-2-1 Doctor u 7-3-1	Cleaning and disinfecting the surfaces Leather part unit	225 226 227 227
7–1 7–2	Exterior. 7-1-1 Chair 7-2-1 Doctor to 7-3-1 7-3-2	Cleaning and disinfecting the surfaces Leather part	226 226 227 227 227
7–1 7–2	Exterior. 7-1-1 Chair 7-2-1 Doctor L 7-3-1 7-3-2 7-3-3	Cleaning and disinfecting the surfaces Leather part Init Touch panel Silicone mat/Handpiece rest Handle cover	226227227227227
7–1 7–2	Exterior. 7-1-1 Chair 7-2-1 Doctor to 7-3-1 7-3-2 7-3-3 7-3-4	Cleaning and disinfecting the surfaces Leather part Init Touch panel Silicone mat/Handpiece rest Handle cover Waste container holder	226227227227227227
7–1 7–2	Exterior. 7-1-1 Chair 7-2-1 Doctor to 7-3-1 7-3-2 7-3-3 7-3-4 7-3-5	Cleaning and disinfecting the surfaces Leather part Init Touch panel Silicone mat/Handpiece rest Handle cover Waste container holder Instrument holder	226226227227227228228
7–1 7–2	Exterior. 7-1-1 Chair 7-2-1 Doctor to 7-3-1 7-3-2 7-3-3 7-3-4 7-3-5 7-3-6	Cleaning and disinfecting the surfaces Leather part	226226227227227228228238
7–1 7–2	Exterior. 7-1-1 Chair 7-2-1 Doctor L 7-3-1 7-3-2 7-3-3 7-3-4 7-3-5 7-3-6 7-3-7	Cleaning and disinfecting the surfaces Leather part	226227227227227228228238238
7–1 7–2	Exterior. 7-1-1 Chair 7-2-1 Doctor to 7-3-1 7-3-2 7-3-3 7-3-4 7-3-5 7-3-6 7-3-7 7-3-8	Cleaning and disinfecting the surfaces Leather part Init Touch panel Silicone mat/Handpiece rest Handle cover Waste container holder Instrument holder BT14 3WAY syringe SYR-20 3WAY syringe 77-type 3WAY syringe	226226227227227227228238238
7–1 7–2 7–3	Exterior. 7-1-1 Chair 7-2-1 Doctor to 7-3-1 7-3-2 7-3-3 7-3-4 7-3-5 7-3-6 7-3-7 7-3-8 7-3-9 7-3-10	Cleaning and disinfecting the surfaces Leather part	226226227227227228238238238
7–1 7–2 7–3	Exterior. 7-1-1 Chair 7-2-1 Doctor to 7-3-1 7-3-2 7-3-3 7-3-4 7-3-5 7-3-6 7-3-7 7-3-8 7-3-9 7-3-10	Cleaning and disinfecting the surfaces Leather part	226226227227227228228238238238
	Exterior. 7-1-1 Chair 7-2-1 Doctor L 7-3-1 7-3-2 7-3-3 7-3-4 7-3-5 7-3-6 7-3-7 7-3-8 7-3-9 7-3-10 Cuspido	Cleaning and disinfecting the surfaces Leather part	226226227227227228228238237238238
7–1 7–2 7–3	Exterior. 7-1-1 Chair 7-2-1 Doctor L 7-3-1 7-3-2 7-3-3 7-3-4 7-3-5 7-3-6 7-3-7 7-3-8 7-3-9 7-3-10 Cuspido 7-4-1	Cleaning and disinfecting the surfaces Leather part	226226227227227227228238237238238239239

		7–4–4	Washing and sterilizing the vacuum handpiece and saliva ejector handpiece	243
		7-4-5	Vacuum line / Saliva ejector line	246
		7-4-6	BT14 3WAY syringe	246
		7-4-7	SYR-20 3WAY syringe	246
		7-4-8	77-type 3WAY syringe	246
		7-4-9	Sensor window for cupfiller	246
		7–4–10	Cuspidor bowl	247
		7-4-11	Solid collector	249
		7-4-12	Spittoon valve	250
		7–4–13	Air filter	251
		7-4-14	Air compressor	251
		7–4–15	Vacuum pump	251
	7–5	How to	detach battery of the doctor unit	252
	7–6	Maintena	ance and inspection	254
		Notes or	n daily maintenance and inspection (by the user)	254
		Notes fo	r periodic inspection	256
	7–7	Detacha	ble parts	257
	7–8	Storage	method	257
8	Mai	intena	nce by Service Engineers	
	8–1	After-sal	es service	258
	8–2	Service I	life	258
	8–3	Period o	f Parts Retention	258
^				
9	Iro	ublesh	nooting	
	9–1	Troubles	hooting	259
	9–2	Message	e on the touch panel and measures to be taken	260
10	۸		ise and Canaumahlas	
10	ACC	essor	ies and Consumables	
	10–1	Accesso	ories	263
	10-2	Consum	nables	263

1–1 Intended Purpose of the Product

This product is an active therapeutic device intended for the exclusive use for diagnoses, treatments and relative procedures of dentistry.

The product must be operated or handled by the qualified dentists or by dental staffs under the supervision of the dentist.

Such dentists or dental staffs should instruct and/or assist the patients to approach to and leave from the product.

Patients should not be allowed to operate or handle the product unless he/she is so instructed.

The product is supplied together with the handpieces like electric micromotor, air turbine and/or motor, scaler and so on.

1–2 Compliance with Regulation and Directive

This product complies with MDR (EU) 2017/745, RoHS Directive 2011/65/EU, and RE Directive 2014/53/EU.

1–3 Declaration of Conformity

We declare under sole responsibility that the device listed below is in conformity with the MDR (EU)2017/745, RoHS Directive: 2011/65/EU based on category 8 of Annex I, and, if applicable, with any other relevant Union legislation that provides for the issuing of an EU declaration of conformity.

Product Type: DENTAL UNIT AND CHAIR (CLASS IIa)

Product Name: EURUS S8

"CLASS IIa" is defined by the rule 9 of MDR Annex VIII.

The product has been designed and manufactured in accordance with the European standards as listed in the Declaration of Conformity.

1–4 How to Dispose of the Device

When disposing of this product and parts replaced, carefully take infection control measures and handle them properly in accordance with the relevant laws and regulations (applicable regulations and local regulations). In the EU area, EU Directive 2012/19/EU (Directive on Waste Electrical and Electronic Equipment [WEEE Directive]) applies to this product. Environment-conscious recycling/disposal is mandatory under this Directive. Remove all batteries when disposing of the product.

Batteries are located inside the wireless foot controller and doctor unit.

Depending on specification a battery inside the doctor unit may not be installed.

Please remove it if it is installed.

[Reference] How to detach battery of the doctor unit [pages 252, 253] [Reference] How to replace batteries of the wireless foot controller [page 148]

1–5 Disposal of Residues

Ask a professional to dispose of amalgam residues.

1–6 A notice to the user and/or patient

Any serious incident that has occurred in relation to the device should be reported to the manufacturer and the competent authority of the Member State in which the user and/or patient is established.

1-7 Compatible Handpieces

Select a handpiece from the list of compatible handpieces. (For reference, see page 38.)

The connectors of our handpiece hose are designed and manufactured in accordance with ISO9168:2009 (DENTISTRY-HOSE CONNECTORS FOR AIR DRIVEN DENTAL HANDPIECES). However, there still could be a case that the connectors of turbines or air motors may not fit into some handpieces due to the manufacturing tolerances. Have your local authorized Belmont dealer to check the connectability before purchasing the handpiece.

Except for our recommended handpieces, we shall not be liable for any problems deriving from bad connectability or their performance.

1–8 Compatible Dental Lights

Select a dental light from the list of compatible dental lights. (For reference, see page 38.)

1-9 Symbols

The symbols listed below are used on this product, on labeling, and in this booklet. Check the meaning of each symbol.

	Switch (ON)	0	Switch (OFF)
(Switch for raising the chair/headrest	(Switch for lowering the chair/headrest
L	Switch for reclining the backrest/headrest	N.	Switch for raising the backrest/headrest
	Switch for changing to the chair/headrest	IP	Switch for returning to the last position
0	Automatic return switch	1	Preset switch 1
2	Preset switch 2	8	Dental light switch ON/ OFF
ョョ	Cupfiller switch/flow control	ST.	Bowl flush switch/flow control
#	Extra switch	∠ ↑ 7	Stick switch for headrest (electrohydraulic)
× · . 7	Stick switch for manual operation	1 LP 2	Stick switch for automatic operation
\I/ 7 F	Service coupler for water use	₩ 1 5	Water flow control of service coupler for water use
\/ 1 F	Service coupler for air use	w 🚈 A	Water/air flow control of syringe spray
炒	Water flow control of handpiece spray	<u></u>	Draining water from air filter
	Protective earthing	<u></u>	Functional earthing
\triangle	Caution *The base color is yellow.	\wedge	General warning sign *The base color is yellow.

\Diamond	Generally prohibited activity		Disassembly, repair or modification prohibited
0	Instructions for mandatory actions in general		Follow instructions for use *The color of black part is blue in the actual label.
†	Type B Applied Parts contacting the patient's body surface only	~	Alternating current
135°C {	An autoclave symbol that indicates parts can be sterilized in an autoclave at temperatures up to 135°C	Ŷ	USB terminal
₩	Manufacturing date and country	SN	Serial number
Ů	Switch for selecting the patient's memory (Adult Mode)	Ť	Serial number
	Switch for selecting the patient's memory (Elderly Mode)	₹ A	Switch the user memory
(B)	Dental light switch ON		Dental light switch OFF
	Timer switch		Cupfiller switch ON
1	Cupfiller switch OFF	i i	Bowl flush switch ON
L 4	Bowl flush switch OFF		Function switch
Manual	Light change switch	Manual Manual Sensor	Sensor/switch mode
Manual only	Switch mode	ON . Keep light ON	ON mode
OFF . Keep light OFF	OFF mode	1	Lock switch (unlocked)
Î	Lock switch (locked)	[™] Heater	Water heater switch ON

∭ Heater ☐ OFF	Water heater switch OFF		Handpiece No. picked up
∭ High	Handpiece heater switch High	∭ Low	Handpiece heater switch Low
S OFF €	Handpiece heater switch OFF	70	Wireless foot controller indicator (paired)
*S	Wireless foot controller indicator (not paired)	05:00 •	Flushing status for handpiece (flushing in progress)
^ ^ V V	Page feed		Flushing status for cupfiller and bowl (flushing in progress)
•	Start		Pause
×	Cancel	III) A	Spray change switch, Air ON
	Spray change switch, Air OFF	w	Spray change switch, Water ON
W	Spray change switch, Water OFF		Handpiece light switch (ON)
*	Handpiece light switch (OFF)	4	Bell switch
^	Select switch (e.g. brightness of handpiece)	<u>∞</u> ② <u>۵</u>	Show the menu
0	Micromotor rotation switch for normal rotation (clockwise)	Rev	Micromotor rotation switch for reverse rotation (counterclockwise)
Reciprocal mode	Reciprocal mode switch for micromotor	Ø	Micromotor rotation switch for reciprocal mode
+	+/- switch	♦	Store switch
AUTO 5 B.O _{Ncm}	Torque control switch	₽ Va	Slide mode change switch Slide mode Va

₽ Fix	Slide mode change switch Slide mode Fix	AUTO S Rev 25	No automatic reverse setting
AUTO 5	Automatic reverse setting	AUTO5)	Automatic forward setting
1:1	Gear ratio change switch		Home switch
<u>5</u>	Return switch	Skip	Skip switch
	Name registration switch	[123]	Alphanumeric switch
	Backspace switch		Chair preset copy
	Handpiece setting copy		Alarm volume
	Touch bar graph		Alarm sound switch (active)
Image: Control of the	Alarm sound switch (muted)	♪ 3	Alarm sound type
Ŧ	Overheat prevention activate	<u> </u>	Chair lock indicator (chair is locked!)
?	Explanation page	(¶*)	Flushing, Washing the vacuum line
M	Vacuum/saliva ejector	ð	Indication of cleaner
	Separate collection of electrical and electronic equipment	for battery	Separate collection of all batteries
REF	Catalog number	EC REP	European Authorized Representative
CH REP	Swiss Authorized Representative	C E 0197	Third-party certification stipulated in Medical Device Regulation: 2017/745

***	Name and address of the manufacturer	R.I.	Rated input
R.V.	Rated voltage	•	Dental patient chair
	Dental Unit	MD	Medical device
(i)	Electronic instructions for use	②	Maximum activation time Non-continuous operation Duty cycle
Ow	Implant switch	Dim	Implant motor
NaCI	Saline irrigation toggle switch ON	NaCl	Saline irrigation toggle switch OFF
	Saline irrigation volume toggle switch at Lv. 5		Saline irrigation volume toggle switch at Lv. 4
	Saline irrigation volume toggle switch at Lv. 3	000	Saline irrigation volume toggle switch at Lv. 2
00	Saline irrigation volume toggle switch at Lv. 1	BOTTLE AIR ON OFF	Water supply toggle switch for water bottle ON: Enable water supply OFF: Stop water supply
BOTTLE AIR PUSH ON PULL OFF	Water supply toggle switch for water bottle PUSH: Enable water supply PULL: Stop water supply	WATER PUSH C ITY PULL BOTTLE	Water supply toggle switch PUSH: Water supply from city water PULL: Water supply from water bottle
	Flushing		Timer switch for flushing
	Flushing settings		Handpiece mode switch
<u></u>	Cupfiller flush mode switch	西口河	Cupfillier, cuspidor bowl flush mode switch
(00:10) 普	Flushing status for cupfiller (flushing in progress)		

1-10 Technical Description

The following are explained in the documents listed below:

Item	Document
How to install this product	Installation instructions Pre-installation instructions
Wiring/plumbing	Installation instructions

2–1 Risk Level Interpretation

Precautions before use

Make sure to carefully read the Safety Precautions and Operating Precautions and use the product correctly.

These precautions are intended to ensure the safe use of the product and prevent harm or damage to users or other people.

According to the magnitude of harm and damage and the degree of urgency, an incident that may be caused by misuse of the product is classified into one of the following categories: CONTRAINDICATION, WARNING, and CAUTION.

All of these categories are important for safety. Always follow the instructions provided.

We assume no responsibility for any accident due to failure to follow the Safety Precautions or Operating Precautions even in the event of harm or damage to users or other persons.

In such case, users or other persons who use the product without observing the Safety Precautions and Operating Precautions are responsible for any harm or damage incurred.

The graphical symbols are explained in detail below.

Once you have fully understood this explanation, read the text.

Classification by degree of harm or damage and urgency

CONTRAINDICATION

Use of the product without regard to this indication will create a hazardous condition that may result in death or serious injury.



WARNING

Improper handling of the product without regard to this indication will create a hazardous condition that may result in death or serious injury.



CAUTION

Improper handling of the product without regard to this indication will create a potentially hazardous condition that may result in moderate or slight injury or property damage.

The following graphical symbols are used to explain your responsibilities for using the product safely:

Graphical symbols for prohibited activity



Generally prohibited activity



Disassembly, repair or modification prohibited

Graphical symbol for mandatory instructions



Instructions for mandatory actions in general

2-2 Safety Precautions

facilities or elevators.

interference waves.

Precautions regarding installation

CONTRAINDICATION

Installing or transferring the product



Use and maintenance of the product



Do not use the equipment in an explosive atmosphere (e.g., in the presence of inflammable gases).

Malfunction of this product may occur in the presence of electromagnetic

Do not install the product near electromagnetic sources such as communication

Improper use in such an atmosphere may cause injury or fire.

Use with caution in the presence of electromagnetic waves.

Do not use equipment generating electromagnetic waves, such as mobile phones, around this product.

Malfunction of this product may occur.

Be sure to turn off the main switch of the product when HF surgical equipment is in use.

Be sure to turn off the main switch when HF surgical equipment is in use because the noise generated from HF surgical equipment may cause incorrect operation of this product.

Never disassemble, repair or modify the product.

Individuals other than your local authorized Belmont dealer should not disassemble or repair this product.

This could lead to an accident, failure, electric shock, or fire. Never modify the product as it is extremely dangerous.





Installing or transferring the product

0

Precautions for installation

Ask your local authorized Belmont dealer to install the product.

Make sure to place the product on a firm and flat floor. Placing the equipment on a non-flat floor may cause it to fall.

Be sure to ground the product securely. (Ask a professional to ground the product.)

Failure or electric leak may result in electric shock.

To avoid the risk of electric shock, this equipment must only be connected to a supply mains with protective earth.

Use and maintenance of the product



Keep moving parts of the product away from patients' and users' hands, fingers, and bodies.

Hands, fingers or bodies may become caught in the product, causing injury.

The patient must not lie on his/her stomach, kneel in the formal seiza position (with his/her buttocks on his/her heels), or sit on the product with a child in his/her arms.

The chair may move unexpectedly, causing injury.

The patient must not sit on the edge of the seat.

The chair may fall or move unexpectedly, causing injury or damage to peripheral devices.

The patient must not sit in an area other than the designated location.

Excessive load must not be applied to the product.

The patient must not sit on the headrest, armrest, or backrest.

This may cause injury due to falling, or damage to peripheral devices.

Excessive load must not be applied to the doctor arm or assistant arm.

The patient must not sit on the doctor arm or assistant arm.

This may cause injury due to falling, or damage to peripheral devices.

A load exceeding the weight limit (3 kg) must not be applied to the doctor table.

This may cause damage or injury.

A load exceeding the weight limit (1.5 kg) must not be applied to the sub-tray of the doctor table (Rod).

This may cause damage or injury.

A load exceeding the weight limit (1.5 kg) must not be applied to the assistant tray.

This may cause damage or injury.



Do not wash the product with water.


This may cause failure or electric shock.




Points to remember when a patient sits on the chair

As shown in the figure, instruct the patient to sit on the chair. Ensure that the patient maintains the posture shown in the figure before operating the chair.







For a young child, confirm that the buttocks are placed on the seat before raising the backrest.

The child might slide down while the chair is moving, resulting in injury.

Pay attention to patients and children.

Keep your eyes on the patient when this product is in use.

Patients (especially children) may touch the control switch or system inadvertently, leading to an accident due to incorrect operation of the product.

Keep children away from this product except when giving treatment.





Precautions for getting on and off EURUS

When the patient gets on or off EURUS, the chair should always be at the lowest position and each operation must be locked by the lock switch.

Before moving a patient from a wheelchair to EURUS or vice versa, ensure that no obstacles (e.g., foot controllers) are situated around the wheelchair or the caregiver.

Contact of the feet or the wheelchair castors with obstacles (such as foot controllers) may cause injury or damage to peripheraldevices.

When the patient is moved from a wheelchair to EURUS or vice versa, he/she must be carefully monitored to prevent falling.

If the patient has to get off EURUS at a position other than the designated position for getting on and off EURUS due to power failure or in the event of an emergency, he/she must be carefully monitored to prevent falling.

Remove the patient's glasses and any accessories (such as a necklace or bracelets) before treatment.

Failure to follow this instruction may hamper treatment and lead to an accident.

Precautions when raising/lowering the backrest

Before lowering the backrest, ensure that the patient's arm or hand is not sandwiched between the backrest and the seat.

Before raising the backrest, ensure that the patient's arm or hand is not sandwiched between the backrest and the armrest.

Precautions for operating the chair and automatic operation

Before and during the chair operation, pay close attention to the operation range (seat raising/lowering direction and backrest lowering/raising direction), and ensure that the chair does not contact any body parts, hands or feet, or obstacles. Body parts, hands or feet, or objects may become caught in the chair, causing injury or damage to peripheral devices.

Before operating the chair, ensure that the patient is sitting in the correct position, and keep your eyes on him/her when the chair is in use.

Precautions when using the headrest (manual)

During the headrest operation, ensure that your fingers do not become caught in the control lever and are not sandwiched between the headrest and the backrest.





Precautions when using the headrest (electrohydraulic)

Before operating the headrest, ensure that the patient is sitting in a normal position and keep your eyes on him/her when the chair is in use. [Reference] Points to remember when a patient sits on the chair [page 20]

Do not use the headrest at an angle at which the patient feels pain.

Before operating the headrest, ensure that no obstacles are placed around the headrest and make sure that there are no body parts or objects sandwiched between the headrest and the backrest.

When the backrest is reclined while the patient is seated, do not raise or lower the headrest with the patient's head on it.

Pay attention to inadvertent use of wireless foot controllers.

If there is more than one EURUS on the same floor, do not operate a wireless foot controller connected to another product.

Precautions when using a micromotor (NBX, NLXplus, NLX nano) with an anti-heat function

When the anti-heat function is activated, do not turn on the main switch for the power cycle and continue operation. The micromotor may generate heat and cause the burns or motor's damages.

Precautions when attaching the nozzle (syringe)

If the syringe is used with its nozzle not securely attached, it may burst out when spraying water or air, and may harm users or other people. Confirm that the nozzle is securely attached before its use. [pages 233, 236 and 238]

Precautions when syringe falls on the floor (syringe)

If the syringe falls on the floor, check that no malfunction is observed. Then, wipe it off with soft cloth moistened with disinfectant FD366 manufactured by Dürr. It may cause injury if the sharp protrusion is found on the nozzle or body, so stop using the product and contact your authorized Belmont dealer.

Development of subcutaneous emphysema

Cooling air (alone or spray) is released from the chip of the handpiece (micromotor and air turbine/motor). This may cause the patient to develop subcutaneous emphysema, so use cooling air with caution.





Pay close attention to a patient who has a cardiac pacemaker or defibrillator implanted.

If any abnormality occurs, immediately turn off the main switch and discontinue use of the product.

EURUS may affect the function of the pacemaker or defibrillator, leading to an accident.

Prohibition of using this equipment adjacent to or stacked with other electronic equipment

Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.

Prohibition of placing portable RF communications equipment adjacent to this product

Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm(12 inches) to any part of EURUS, including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.

Immediately wipe off any water spillage or leakage on the floor.

Decreased strength of the floor may cause the product to fall, leading to injury or damage to peripheral devices.

Clean the product thoroughly.

Poor cleaning may cause bacteria to grow, posing a health risk. See cleaning procedures on pages 225 to 251.

Be sure to conduct maintenance.

Use of the product without maintenance may cause injury or damage to peripheral devices.

See maintenance information on pages 254 to 256.

Discontinue use of the product if it is broken.

In the case of a broken product, immediately discontinue use and turn off the main switch. Then, ask your local authorized Belmont dealer to repair the product.

Turn off the main switch during cleaning.

Failure to follow this instruction may cause electric shock or ignition. The product may also move unexpectedly, causing injury.

Action taken for power failure

To prevent unexpected operation of the product after recovery from power failure, turn off the main switch and put the handpiece/syringe in the instrument holder/assistant holder.





Be sure to turn off the breaker for devices when the product is not used for a long period of time.

Make sure to turn off the breaker for devices in a clinic when the product is not used for a long time for reasons such as closing time and non-consultation day. If the breaker is not turned off, a fire may be caused by a leakage of electricity due to insulation deterioration.





Do not allow a person who exceeds the weight limit to sit on the chair.

Falling or operational failure may occur.

[Reference] Weight limit

4 Product Specifications, 4-1 Technical Data [page 44]

Do not hit or rub the product.

This may cause damage to the cover or operational failure.

Use a battery specified by Belmont only for the wireless foot controller.

Do not combine a new battery with an old one and do not use different types of batteries (e.g., an alkaline battery and a nickel-hydrogen battery). Improper use of batteries may lead to battery leakage or rupture.

Do not touch leakage from a battery.

Contact of battery fluids with the eyes may result in blindness. Rinse with clean water immediately without rubbing, and consult a physician promptly.

Contact of battery fluids with the skin may cause skin disorders, so immediately rinse with clean water.

Ensure that each part operates normally, with no abnormalities detected, before operation.

Always inspect the product for abnormal findings such as loose components, backlash, tilting, vibration, sound, abnormal temperature, or bad odors. If you feel something is wrong, immediately discontinue use of the product and turn off the main switch. Then, contact your local authorized Belmont dealer.

Read the accompanying documents for each device.

Before use, make sure to carefully read the instructions for use supplied with each device and use the device correctly.

Be sure to operate switches manually.

Make sure to operate the switches manually, except for the foot controller operated by the foot and stick switches. Failure to operate the switches by hand may cause damage or malfunction.

Carefully operate the switches to prevent a mistake.

The operator should pay close attention to people around the product and say something before operation to prevent any errors.

Peel off the film attached to the touch panel before initial use Using the touch panel with the film attached may lead to incorrect operation, resulting in injury.







Precautions when cleaning the touch panel

To clean and disinfect the touch panel, use ethanol for disinfection. Using other disinfectant may lead to incorrect operation, resulting in injury.

Be certain to wipe off all water and detergent. Otherwise, it may cause operational failure, malfunction, resulting in injury.

Precautions for moving the doctor unit

Carefully look around while moving the doctor unit. Contact with the chip of the handpiece may cause injury.

Precautions when using the cart

When using the cart within the operation range of the chair, pay attention not to collide with person or chair. Contact with the tip of the handpiece may cause injury.

Do not sit or lean on the cart. Do not step on the cart base or cart hose. Otherwise, such actions may damage the hose or cause the cart to fall resulting in injury.

Precautions when using a handpiece

In the event of heat or smoky smell, stop using the handpiece, turn off the main switch, and contact your local authorized Belmont dealer.


This may cause burns or have an adverse effect on the dental pulp.

Precautions when using an ultrasonic scaler

After use, attach a dedicated cover (if any) to the scaler tip and put it in an instrument holder. Contact with the tip of the scaler may cause injury.

Precautions when using a dedicated function for NLXplus/ MX2

If a reverse-screw-shaped file is attached, make sure to select "No auto reverse function," and change the rotation direction by micromotor rotation switch. If the NLXplus/MX2 is used with "Auto reverse function/Auto forward function" selected, the file will be damaged, causing injury.



Do not use the handpiece with its hose twisted

Repeated actions of picking up and returning the handpiece may cause its hose twisted.

Check the hose periodically to see if it is not twisted. If twisted, unwind it before

Continual use of the handpiece with its hose twisted will cause the kinks in the hose or breaking of the wire, making the handpiece unusable.





Precautions for armrest rotation

Ensure that no obstacles are placed around the armrest and fingers do not become caught in the armrest.

Do not operate the chair when the armrest is rotated. Before operating the chair, return the armrest to its original position.

Precautions when using a monitor bracket

Do not apply excessive load to or make an impact on a monitor or monitor bracket. Do not mount a monitor if it does not meet the conditions provided below to prevent damage or injury.

Size: Up to 340 x 530 mm (L x W) [22-inch or smaller monitor]

Weight: Up to 6.5 kg

* Excluding dimensions of monitor handle and other accessories

Precautions when handling batteries

Remove the battery from the wireless foot controller when it is not used for more than a week.

Turn off the main switch during battery replacement. If not, and a switch or pedal may be pressed mistakenly, it will lead to incorrect operation of the product and may cause any damage to the person or property.

Put on the cleaning gloves when detaching cuspidor bowl. Cuspidor bowl is made of ceramic that might cause injury when broken.

Precautions for right/left handed conversion

Make sure to read through pages 160-167 for instructions before performing the right and left handed conversion.

If the conversion is performed without reading, it may cause physical injury or property damage.

Take care so the doctor table does not hit the cuspidor unit during the conversion.

Take care not to pinch the vacuum hose and saliva ejector hose between the assistant arm and the cuspidor swing arm during the conversion.

Immediately wipe off any chemical solutions or water adhered to EURUS.

Adherence of chemical solutions or water to the control unit may cause operational failure or electrical leak. If chemical solutions or water are adhered, immediately turn off the main switch and wipe them off with a dry, soft cloth.

Close the main water valve at the end of day.

To prevent the water leakage, make sure to close the main water valve at the end of day.

Turn off the main switch at the end of day or during a recess. Malfunction due to contact with EURUS will cause damage or injury.

Clean and sterilize the HVE tip, syringe nozzle before use.

The HVE tip, syringe nozzle which contacts oral tissues, is provided without sterilization.

Cleaning and sterilization is necessary before use.



Safety precautions regarding Conduct flushing before treatment. water quality



If this product is not used for a long time, water retained in ducts and in the water heater will be susceptible to bacterial growth. To provide safe treatment and operate the handpiece without any trouble, never forget to perform flushing (discharge) of the water lines before starting treatment.

After morning and evening treatments, it is recommended to conduct flushing with fresh water for at least 2 minutes and 40 seconds(it may differ depending on water quality) to prevent bacteria growth.

Time required for standard flushing of the unit water lines

Flushing water circuits of handpieces	40 seconds to 2 minutes 40 seconds
Air turbine / Micromotor / Air motor / Ultrasonic scaler /	
Syringe	

Filling the water circuits of the handpieces with chemical solution Filling the water circuits of the cupfiller with chemical solution	30 seconds to 10 minutes
Air turbine / Micromotor / Air motor / Ultrasonic scaler / Syringe +	20 seconds to 5 minutes
Cupfiller	10 seconds to 5 minutes

Flushing the water circuits of handpieces Flushing the water circuits of cupfiller and cuspidor bowl	5 minutes 20 seconds to 10 minutes
Air turbine / Micromotor / Air motor / Ultrasonic scaler / Syringe +	2 minutes 40 seconds to 5 minutes
Cupfiller Bowl flush	2 minutes 40 seconds to 5 minutes

Vac Pac unit type / without cuspidor bowl type			
Flushing the water circuits of handpieces			
(Short mode)	40 seconds to 2 minutes 40 seconds		


Vac Pac unit type / without cuspidor bowl type		
Flushing the water circuits of handpieces		
(Long mode)	2 minutes 40 seconds to 5 minutes	


Time required for standard washing for the vacuum line

Rinsing the vacuum line	4 minutes
Washing the vacuum line with cleaner	4 minutes
Rinsing the vacuum line+washing the vacuum line with cleaner	8 minutes


[Reference] Selection and implementation of flushing method [pages 171 to 190]

Base mount





Swing mount

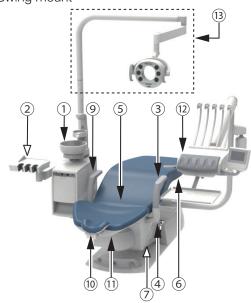

Points to remember when operating the product

Meaning of a symbol



Point to remember

(locations requiring attention including moving parts, rotating parts, and detachable parts)



Point to remember where an emergency stop mechanism is available

Meanings of each point to remember

- ① Pay attention to prevent contact with the cuspidor bowl. When the cuspidor bowl is rotated to the side of the chair, keep it away from the armrest and the patient.
- ② Pay attention to prevent contact with the assistant holder.
 The upper part of the patient's body should not lean forward over the cuspidor unit.
- ③ Pay attention to prevent body parts or objects from becoming caught in the armrest (when rotating).
 - Do not operate the chair when the armrest is rotated.
- 4 Pay attention to prevent body parts or objects from becoming caught in the armrest (when lowering the chair).
 - Do not place the body parts or objects at the the armrerst bracket when lowering the chair.
- ⑤ Pay attention to prevent body parts or objects from becoming caught in the backrest moving parts.
 - Do not sandwich your hands or feet between the backrest and the seat.
- ⑤ Pay attention to prevent body parts or objects from becoming caught in the bottom of the seat.
 - Do not place your hands or feet in the bottom of the seat.
- Pay attention to prevent body parts or objects from becoming caught in the rear link cover.
 - Do not place the body parts or objects between the rear link cover and base plate.
- ® Pay attention to prevent body parts or objects from becoming caught in the flange cover
 - Do not place the body parts or objects between the flange cover and base plate.
- Pay attention to prevent body parts or objects from becoming sandwiched between the cuspidor and the chair.
 - Before operating the chair, ensure that no hands, feet, or obstacles are placed between the cuspidor and the chair.
- Pay attention to prevent body parts or objects from becoming caught in the headrest moving part.
 - Ensure that your fingers and hair do not become caught in the headrest moving part.
- ① Pay attention to prevent contact with the backrest.


 Before operating the backrest, ensure that no obstacles are placed around the
- ② Pay attention to prevent contact of the chair with the doctor unit.Do not place the doctor unit within the operational range of the chair.
- (3) Pay attention to prevent contact with the light.
 The light should not be placed near people or surrounding obstacles.
- (4) Pay attention to prevent contact of the chair with the cart.Do not place the cart within the operation range of the chair.



WARNING

When operating the chair, do not place the body parts or objects around the moving parts. This may cause injury.

Base mount Vac Pac 1 9 10 6 3 5 Cart Vac Pac 1 8 4 2 13

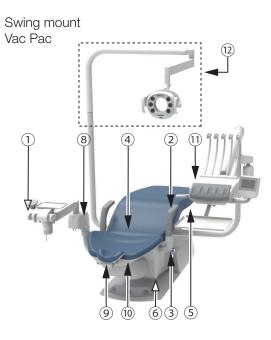

Points to remember when operating the product

Meaning of a symbol



Point to remember

(locations requiring attention including moving parts, rotating parts, and detachable parts)



Point to remember where an emergency stop mechanism is available

Meanings of each point to remember

- Pay attention to prevent contact with the assistant holder.

 The upper part of the patient's body should not lean forward over the cuspidor unit.
- ② Pay attention to prevent body parts or objects from becoming caught in the armrest (when rotating).
 - Do not operate the chair when the armrest is rotated.
- 3 Pay attention to prevent body parts or objects from becoming caught in the armrest (when lowering the chair).
 - Do not place the body parts or objects at the the armrerst bracket when lowering the chair.
- 4 Pay attention to prevent body parts or objects from becoming caught in the backrest moving parts.
 - Do not sandwich your hands or feet between the backrest and the seat.
- ⑤ Pay attention to prevent body parts or objects from becoming caught in the bottom of the seat.
 - Do not place your hands or feet in the bottom of the seat.
- ⑤ Pay attention to prevent body parts or objects from becoming caught in the rear link cover.
 - Do not place the body parts or objects between the rear link cover and base plate.
- Pay attention to prevent body parts or objects from becoming caught in the flange cover.
 - Do not place the body parts or objects between the flange cover and base plate.
- ® Pay attention to prevent body parts or objects from becoming sandwiched between the Vac Pac and the chair.
 - Before operating the chair, ensure that no hands , feet, or obstacles are placed between the cuspidor and the chair.
- Pay attention to prevent body parts or objects from becoming caught in the headrest moving part.
 - Ensure that your fingers and hair do not become caught in the headrest moving part.
- (1) Pay attention to prevent contact with the backrest.
 Before operating the backrest, ensure that no obstacles are placed around the
- ① Pay attention to prevent contact of the chair with the doctor unit.

 Do not place the doctor unit within the operational range of the chair.
- ② Pay attention to prevent contact with the light.
 The light should not be placed near people or surrounding obstacles.
- (3) Pay attention to prevent contact of the chair with the cart.Do not place the cart within the operation range of the chair




WARNING

When operating the chair, do not place the body parts or objects around the moving parts. This may cause injury.


2-3 Locations Where Caution Labels Are Attached

Base mount

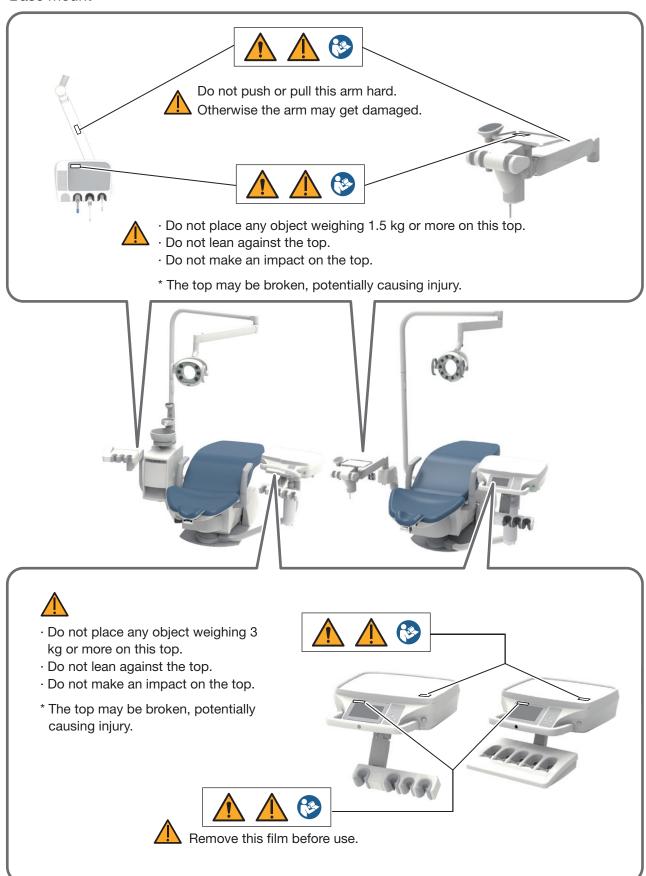


2 Safety Consideration

Cart

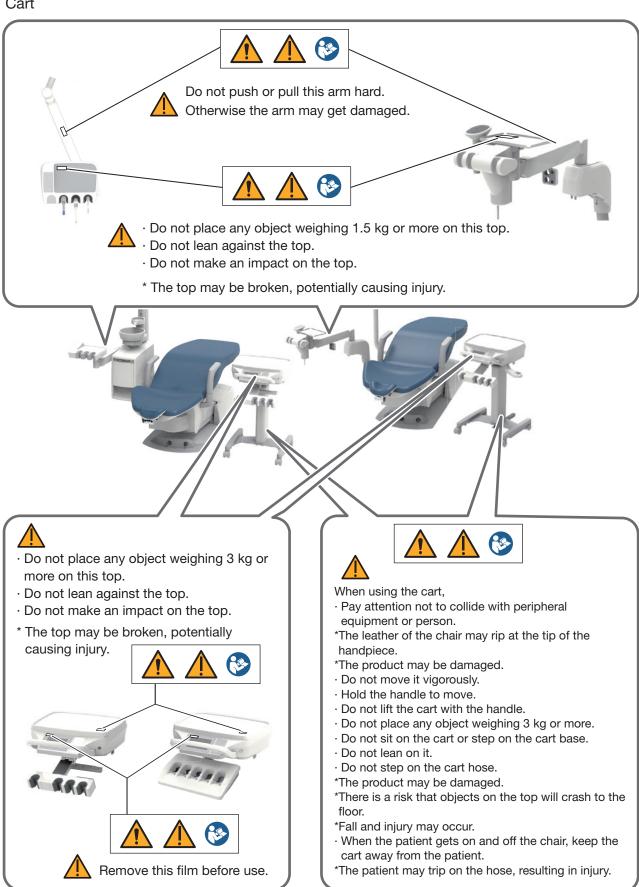

2 Safety Consideration

Swing mount

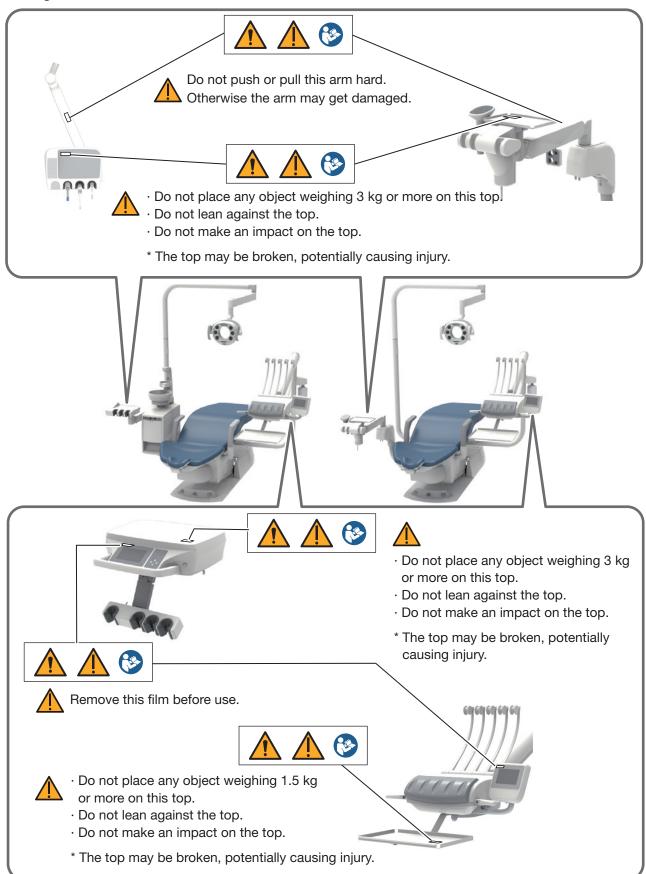

2–4 EMC Information

This product complies with EMC Standard EN 60601-1-2:2015+AMD1:2021.

1. Precautions regarding EMC and compliance with accompanying documents

Medical electrical equipment requires special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in this booklet.

2. Effects of RF communication devices

Portable and mobile RF communication devices can affect medical electrical equipment.

3. Installation exclusion environment

Hospitals except for near active HF SURGICAL EQUIPMENT and the RF shielded room of an ME SYSTEM for magnetic resonance imaging, where the intensity of EM DISTURBANCES is high.

4. Electromagnetic emission declaration

Guidance and manufacturer's declaration-electromagnetic emissions			
EURUS is intended for use in the electromagnetic environment specified below. The customer or user of EURUS should ensure that it is used in such an environment.			
Emissions test	Compliance		Electromagnetic environment —
Emissions test	Japan	CE	guidance
RF emissions CISPR 11	Group 1		EURUS only uses RF energy for its internal functions. Therefore, its RF emissions are very low and are not likely to cause any interference with nearby electronic equipment.
RF emissions CISPR 11	Class B		EURUS is suitable for use in
Harmonic emissions IEC 61000-3-2	Not applicable	Class A	all establishments, including domestic establishments and those directly connected to the
Voltage fluctuations/ Flicker emissions IEC 61000-3-3	Not applicable	Complies	public low-voltage power supply network that supplies buildings used for domestic purposes.



Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation.

If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.

2 Safety Consideration

5. Electromagnetic immunity declaration 1

o. Licotioinagi	ictic irriiridriity	accidiation i	
Guidance and manufacturer's declaration—electromagnetic immunity			
EURUS is intended for use in the electromagnetic environment specified below. The customer or user of EURUS should ensure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±8 kV contact ±15 kV air	±8 kV contact ±15 kV air	Flooring should be wood, concrete, or ceramic tiles. If the floor is covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/ output lines	±2 kV for power supply lines ±1 kV for input/ output lines	The mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1kV differential mode ±2kV common mode	±1kV differential mode ±2kV common mode	The mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	0% Ut; 0.5 cycles 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315° 0% Ut; 1cycle and 70% Ut; 25/30 cycles at 0°, single phase 0% Ut; 250/300 cycles	0% Ut; 0.5 cycles 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315° 0% Ut; 1cycle and 70% Ut; 25/30 cycles at 0°, single phase 0% Ut; 250/300 cycles	The mains power quality should be that of a typical commercial or hospital environment. If the user of EURUS requires continued operation during mains power interruptions, it is recommended that EURUS be powered from an uninterruptible power supply or a battery.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30A/m	30A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
Proximity magnetic fields IEC 61000-4-39	134.2kHz 65A/m, Pulse Modulation 2.1kHz 13.56MHz 7.5A/m, Pulse Modulation 50kHz	134.2kHz 65A/m, Pulse Modulation 2.1kHz 13.56MHz 7.5A/m, Pulse Modulation 50kHz	Proximity magnetic fields should be at levels characteristic of a typical location in a professional healthcare facility environment.
Note Ut is the AC	mains voltage prior	to the application	of the test level.

6. Electromagnetic immunity declaration 2

Guidance and manufacturer's declaration—electromagnetic immunity

EURUS is intended for use in the electromagnetic environment specified below. The customer or user of EURUS should ensure that it is used in such an environment.

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment—guidance
Conducted RF IEC 61000-4-6	3V 0.15MHz-80MHz 6V 0.15MHz-80MHz in ISM bands and amateur radio bands	3V 0.15MHz-80MHz 6V 0.15MHz-80MHz in ISM bands and amateur radio bands	Warning: Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of EURUS,including cables specified by the manufacturer. Otherwise,degradation of the performance of this equipment could result.
Radiated RF IEC 61000-4-3	3V/m 80MHz-2.7GHz 80% AM (1 kHz)	3V/m 80MHz-2.7GHz 80% AM (1 kHz)	
Near electromagnetic field caused by RF wireless communication devices IEC61000-4-3	See the table on the next page (page 37)	See the table on the next page (page 37)	

7. Essential performance

Unless operated by the chair control switch, the chair will not make any movements. Unless operated by the foot controller, the handpiece will not move except for sounding a buzzer and switching the indicator on/off. Loss or decline of essential performance may cause the chair or handpiece to move unexpectedly, causing harm or damage to the patient, operator or people or objects around the patient or operator.



Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm(12 inches) to any part of EURUS, including cables specified by the manufacturer.

Otherwise, degradation of the performance of this equipment could result.

2 Safety Consideration

Near electromagnetic field caused by RF wireless communication devices

Test frequency (MHz)	Modulation	IEC 60601 test level	IEC 60601 compliance level			
385	Pulse modulation ^{a)} 18Hz	27V/m	27V/m			
450	Frequency modulation ±5kHz shift 1kHz sine wave	28V/m	28V/m			
710 745 780	Pulse modulation ^{a)} 217Hz	9V/m	9V/m			
810 870 930	Pulse modulation ^{a)} 18Hz	28V/m	28V/m			
1720 1845 1970	Pulse modulation ^{a)} 217Hz	28V/m	28V/m			
2450	Pulse modulation ^{a)} 217Hz	28V/m	28V/m			
5240 5500 5785	Pulse modulation ^{a)} 217Hz	9V/m	9V/m			
Note a) The carrier is modulated by a square wave with a 50% duty cycle.						

2-5 Compatible Handpieces

The following handpieces are compatible with this product:

	BT14 3WAY			
	SYR-20 3WAY			
	77-type 3WAY			
0.1	DCI 3439 3WAY			
Syringe	DCI 3459 3WAY			
	LUZZANI 3WAY (Minimate)			
	LUZZANI 3WAY (Minilight)			
	LUZZANI 6WAY (Minilight)			
Air turbine	NSK (PTL-CL-LED+M900L)			
Air motor	NSK (M205+M65)			
All Motor	NSK (M205+M25L)			
	BIEN AIR MX-i LED 3rd Gen.			
	BIEN AIR MX2 (DMX3)			
Micromotor	BIEN AIR MCX			
MICIOITIOLOI	NSK NLX plus			
	NSK NLX nano			
	NSK NBX			
	NSK VARIOS VS170 SCALER			
	NSK VARIOS VS170 LUX SCALER			
Scaler	DENTSPLY CAVITRON SCALER(TYPE G139)			
Scalei	SATELEC SP4055 NEWTRON			
	SATELEC Xinetic			
	EMS NO PAIN			
Curing light	SATELEC MINI LED STD OEM			
	ACTEON SOPRO 617			
Intraoral camera	ACTEON SOPRO CARE			
	ACTEON C20 Full HD Intraoral camera			
	ACTEON C50 Full HD Intraoral camera			

2-6 Compatible Dental Lights

The following dental lights are compatible with this product:

Dontal light	EURUS LIGHT
Dental light	900 DENTAL LIGHT

3-1 Operating Precautions

Immediately wipe off any chemical solutions adhered to EURUS. Otherwise, they may cause deterioration or discoloration.

Do not apply heat to the product.

This may cause deterioration or discoloration.

Discoloration of resin

Resin materials are used in external components of the product.

Carefully selected materials are used; however, discoloration may occur for reasons such as natural deterioration or the adherence of chemical solutions. To ensure use of EURUS for as long as possible, immediately wipe off any chemical solutions adhered and avoid sunlight.

Do not place objects other than a human being on the seat.

This may cause deformation, tears, or corrosion of the leather.

Check the operation of the doctor table

Moving the doctor table upward/downward without releasing the brake may cause damage to the product.

Be sure to release the brake first by pressing the brake release switch. Then, move the doctor table upward/downward.

Precautions when using the cart

Pay attention not to collide with peripheral equipment. The leather of the chair may rip at the tip of the handpiece or the product may be damaged.

If you do not follow the instructions below, the product may be damaged or there is a risk that objects on the top will crash to the floor.

(Do not move it in rough and vigorous way. /Hold the handle to move it. /Do not lift the cart with the handle. /Do not place any object weighing 3 kg or more. /Do not sit on the cart or step on the cart base.)

Carefully handle handpieces/syringes.

Handle handpieces/syringes with care to prevent dropping. Dropping them may cause damage or deformation.

Illumination of LED indicators

Since illumination of the LED indicators acts as a guide for chair/ handpiece locking, the occurrence of mode switching, ensure that the control switches function normally as displayed before the start of work every day.

3 Precautions for Use

Check the operation of the compressor.

This product will not work unless air is supplied. Switch on the compressor before operating this product.

Pay attention to prevent the use of water other than tap water.

This product is intended for use with tap water, purified water, distilled water, or pure water; use of water other than those mentioned above may lead to failure. If the product breaks down due to the use of unspecified water, it will not be covered by the guarantee.

Action to take in the case of a water leak

In the event of a water leak, close the main water valve, turn off the main switch and breaker for devices used in the clinic, and contact your local authorized Belmont dealer.

Use this product only for dental treatment.

This product is a dental unit and patient chair used for dental treatment. Only a dentist and dental staff are allowed to use this product.

Chair's weight limit

The chair may rise slowly if a person weighs around the maximum lifting capability.

[Reference] Weight limit

4 Product Specification, 4-1 Technical Data [page 44]

3-2 Precautions for Using Synthetic Leathers

Adherence of clothing dye

To clean and disinfect the synthetic leathers, wipe the surface with a soft cloth or paper towel moistened with FD360 manufactured by Dürr, and then wipe it with a dry cloth.

Dye may migrate from clothes or belts to the synthetic leathers of the product. If dye is adhered, wipe gently with a soft cloth impregnated with a neutral detergent diluted to about one-tenth with water as soon as possible to prevent penetration. Next, wipe with water and then thoroughly with a dry cloth.

Pay attention to prevent deterioration and dye migration due to contact.

Contact with other resin materials, coated products, solvents, and adhesive tapes may cause changes in the surface gloss, cracks, deformation or abrasion.

Dye may migrate from newspapers or printed matters to the product.

Dye may migrate from printed clothes such as T-shirts or denim clothes to the leathers of this product.

Adherence of benzene, nail polish remover, alcohol, or oil may cause discoloration, surface dissolution, changes in gloss, hardening, softening or abrasion.

Use of a bleaching agent or a sheet cleaned by bleach may cause changes in gloss or discoloration.

Placing the product near a heat source such as a heater may cause deformation or discoloration.

Shield the product from direct sunlight by using a curtain. Direct sunlight may cause surface change, shrinkage, discoloration or fading.

Placing a heavy object on the product for a long time may leave a mark or wrinkle.

4–1 Technical Data

4-1-1 Specification Variations

S1								
		S8H	S8P	S8CH	S8CP	S8SR	S8SH	S8SP
Chair	Contour	0	0	0	0	0	0	0
	Folding legrest							
Cuspidor unit	Chair mount	0	0	0	0	0	0	0
Vac Pac unit	Chair mount	0	0	0	0	0	0	0
Doctor unit delivery	Base mount	0	0					
	Cart							
	Swing mount					0	0	0
Instrument delivery	Holder	0		0			0	
	Place holder	[0	Ī	0	Ī	Ī	0
	Rod					0		

4-1-2 S8

Model Doctor unit

AU-ER8-CBM (Base mount)

AU-ER8-CT (Cart)

AU-ER8-CSWR/CSWH (Swing mount)

Cuspidor unit AU-ER8-SW* Vac Pac unit AU-ER8-VP* Chair

AC-ER8-CP* (Cart Power Headrest) AC-ER8-CD* (Cart Manual Headrest) (* represents single or multiple strings

or numbers.)

Classification for protection against

electric shock

Class I Equipment

Classification according to the degree of protection against electric shock

Type B Applied Parts

(handpiece/syringe/chair upholstered

parts/armrest)

Classification according to the degree of protection against ingress of water

or particulate matter

Foot controller IPX1

Rated voltage AC230 V

Power frequency 50/60 Hz

Power input 5.5 A

Fuse Fuse holder

Primary circuit: 8A / 250V

(Interrupting capacity: 80A / 250VAC)

Operating speed: Time lag

Size: 5.2 × 20 mm

Secondary circuit for 24V / 6.5A line

10A / 250V

(Interrupting capacity: 1500A / 250VAC)

Operating speed: Time lag

Size: $5.2 \times 20 \text{ mm}$

Secondary circuit for 24V / 5A line

6.3A / 250V

(Interrupting capacity: 1500A / 250VAC)

Operating speed: Time lag

Size: $5.2 \times 20 \text{ mm}$

Secondary circuit for 14V / 5A line

6.3A / 250V

(Interrupting capacity: 1500A / 250VAC)

Operating speed: Time lag

Size: 5.2 × 20 mm

Secondary circuit for handpiece water heater

6.3A / 250V

(Interrupting capacity: 1500A / 250VAC)

Operating speed: Time lag

Size: 5.2 × 20 mm

Secondary circuit for 6-way syringe/cup water supply and

water heater 6.3A / 250V

(Interrupting capacity: 1500A / 250VAC)

Operating speed: Time lag

Size: 5.2 × 20 mm

Power board for NLX Plus/NLX Nano/MX2/MCX

5A / 250V

(Interrupting capacity: 100A / 250VAC)

Operating speed: Time lag

Size: ø8.35 mm

Foot controller control board

0.315A / 32V

(Interrupting capacity: 1.2A / 32VAC) Operating speed: Normal operation

Size: 1.6 × 0.8 mm

Chair control board

1.25A / 250V

(Interrupting capacity: 1500A / 250VAC)

Operating speed: Interrupting

Size: 5.2 × 20 mm

AC/DC power circuit board

2.0A/250V

(Interrupting capacity: 100A/300VAC)

Operating speed: Time lag Size: 8.5x8.5x4 mm

Operation mode Non-continuous operation (motor)

Maximum operating time, 3 minutes

DUTY 1:15

Weight Cuspidor unit 40 kg

Doctor unit

 Base mount
 30 kg

 Cart
 25 kg

 Swing mount
 40 kg

 Vac Pac
 25 kg

 Chair
 170 kg

Main air pressure 0.5 MPa

Main water pressure 0.2 MPa

Chair Initial height/stroke 490 mm/310 mm

Chair raising and lowering mechanism Electrohydraulic

Headrest Electrohydraulic

Manual

Backrest Electrohydraulic

Seat Backrest-linked tilt mechanism

Armrest Left rotated/Right rotated

Angle of rotation 90°/135°

Upholstered parts Synthetic leather

Control switch Stick switch

Usage environment Temperature 0°C to 40°C

Humidity 10% to 95% (No condensation) Atmospheric pressure 700 to 1060 hPa

Transportation/storage environment Temperature -20°C to 70°C

Humidity 10% to 95% (No condensation) Atmospheric pressure 700 to 1060 hPa

Weight limit Doctor table 3 kg

Sub-tray of doctor table (Rod) 1.5 kg

Assistant tray 1.5 kg

Chair (maximum patient mass;) 200 kg


Adaptation to high-oxygen environment
The product is not suitable for use in a


high-oxygen environment.

Refer to the rating plate for the capacity of power supply.


Dimensional drawing (standard values are provided)

Base mount Cuspidor

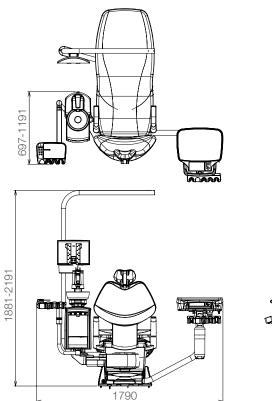



Base mount Vac Pac

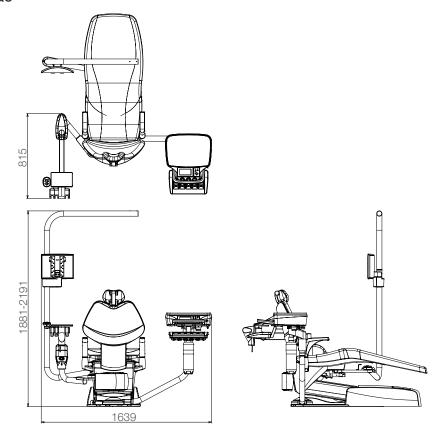


Unit: mm


Tolerance in dimensions: ±10%

Dimensional drawing (standard values are provided)

Cart Cuspidor

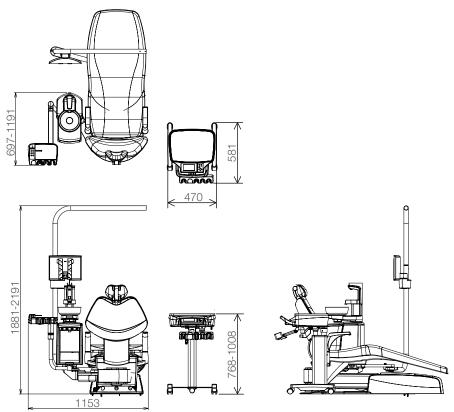


Cart Vac Pac

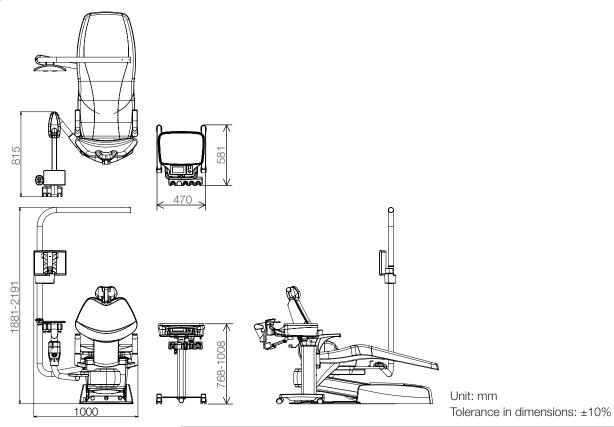


Dimensional drawing (standard values are provided)

Swing mount Cuspidor

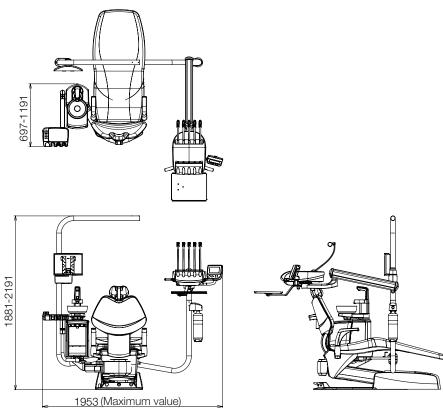

Swing mount Vac Pac

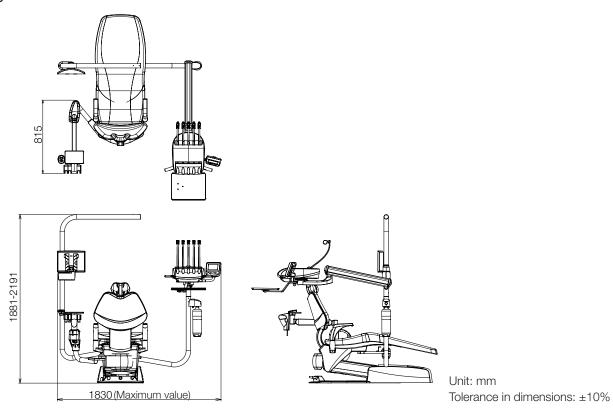


Chair


Dimensional drawing (standard values are provided)

Base mount

Headrest: Electrohydraulic

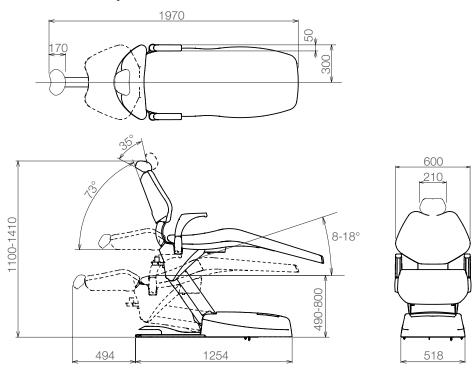


Headrest: Manual

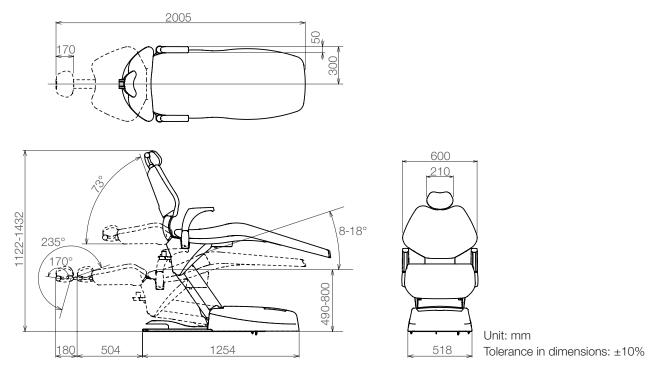


Dimensional drawing (standard values are provided)

Cart

Headrest: Electrohydraulic

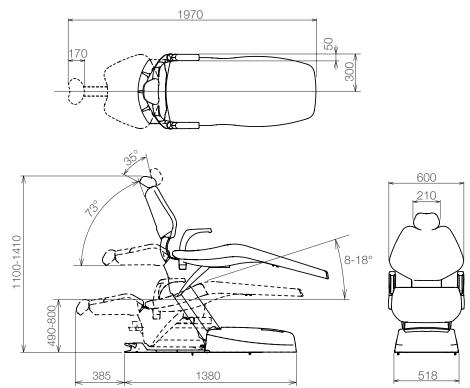

Headrest: Manual

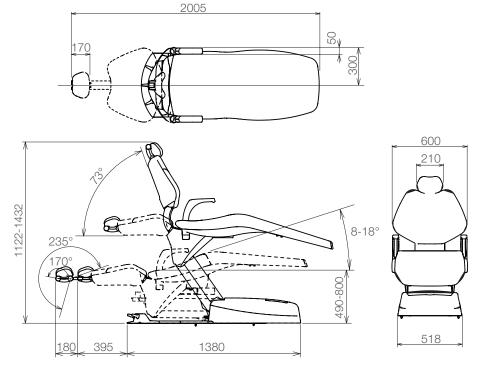

Unit: mm

Tolerance in dimensions: ±10%

4–1–3 Specifications for Air/Water/Suction

Water supply Pressure: 0.2-0.4 MPa

Minimum water flow: 6 L/min Hardness: Less than 2.14mmol/L

(< 12-dH)

pH: 6.5-8.5

Particle water filter: 100 µm

Water quality: Must satisfy the national requirements pertaining to drinking water. Comply with the national requirements concerning the connection of the EURUS unit to the public drinking water supply.

Air supply Pressure: 0.5-0.7 Mpa

Minimum flow rate: 100 L/min

Humidity: 10 to 95% (No condensation) Oil contamination: Max 0.5mg/m³


Particle contamination: Particle size (1 µm - 5 µm),


less than 100/m³
Particle air filter: 5 m

Type of air volume flow rate type 1: high - volume suction system

VH-18 HVE Tip size: Ø11/Ø16

4–2 System Overview Base mount Cuspidor Chair [page 54] Assistant unit [page 61] Doctor unit [pages 57, 58] Cuspidor unit [page 59] Headrest [page 55] Junction unit [page 61] Foot controller [page 56] Base mount Vac Pac Chair [page 54] Vac Pac Doctor unit [page 61] [pages 57, 58] Headrest Junction unit [page 55] [page 61] Foot controller [page 56]

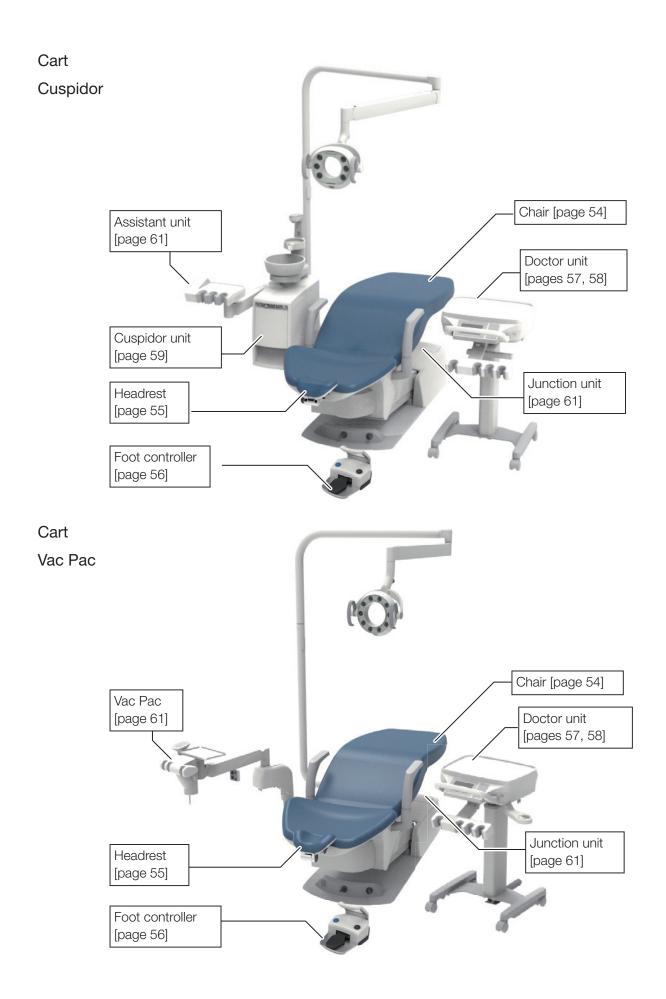

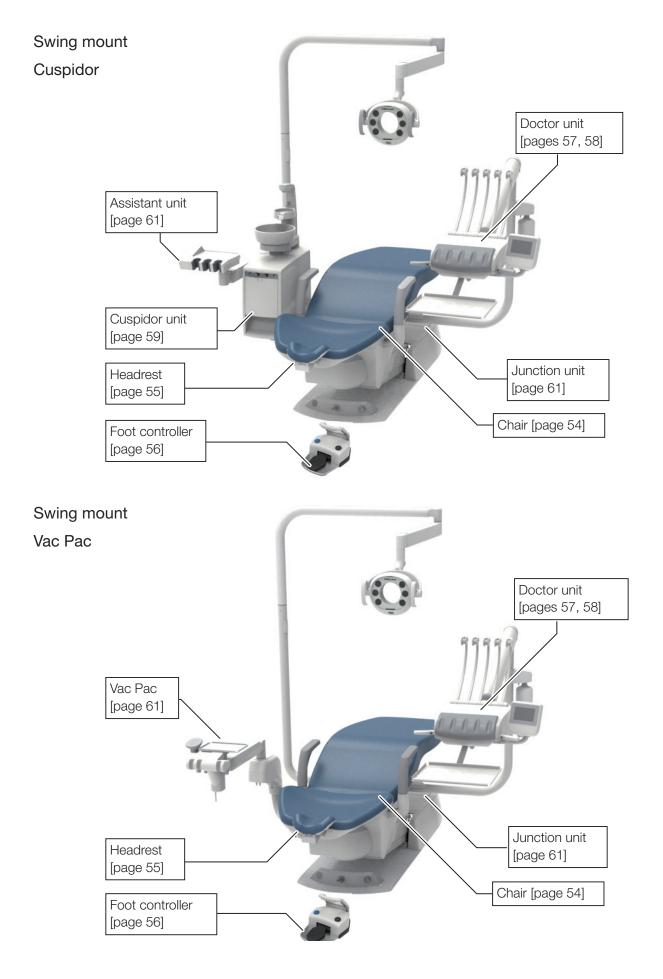

4–3 Name of Each Part

4-3-1 Chair


Base mount

The headrest may differ according to the specifications selected.





Cart / Swing mount

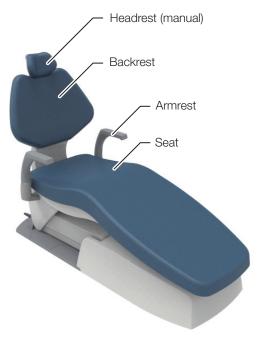




Rear link cover

The headrest may differ according to the specifications selected.

Stick switch
(Three different stick switches are available: For the headrest, for the chair

[manual], and for the chair [auto])




The position or availability of the stick switch may differ according to the specification selected.

4-3-2 Headrest

4–3–2–1 Headrest (electrohydraulic)




4-3-2-2 Headrest (manual)

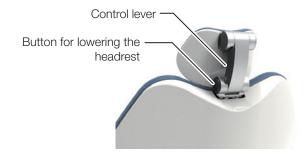


4-3-3 Foot Controller (wired/wireless)

Type 1

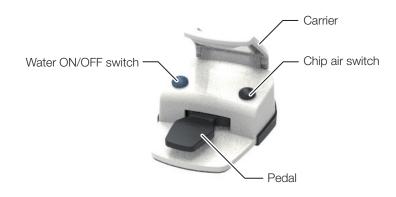

Type 2

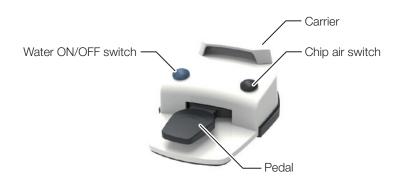

4-3-4 Foot Switch

Type 1



Type 2




4–3–5 Doctor Unit

4–3–5–1 Doctor Unit Delivery


Base mount



Cart

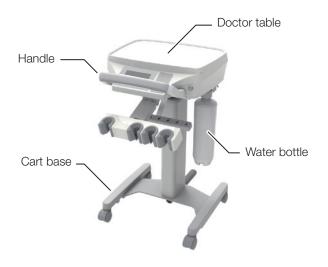


Swing mount

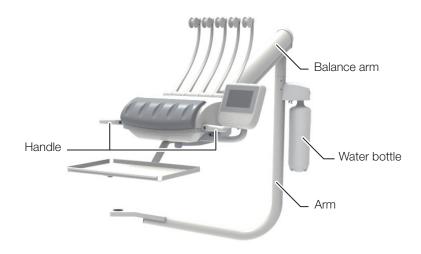


4-3-5-2 Instrument Delivery


Holder

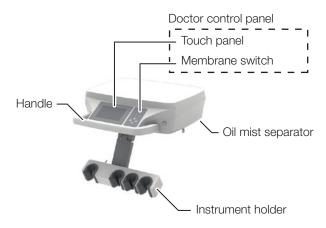


Place holder

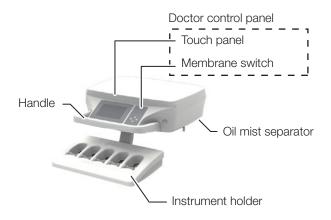

Rod

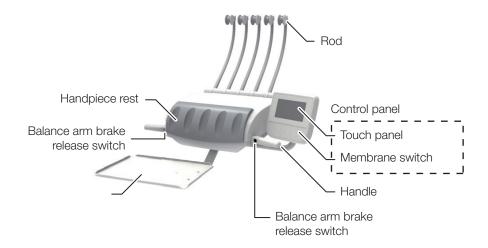

4–3–6 Cuspidor Unit

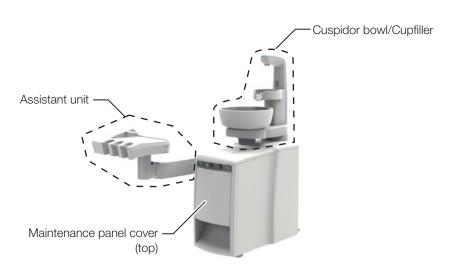





4-3-6-1 Cuspidor bowl/Cupfiller



4-3-6-2 Maintenance Panel

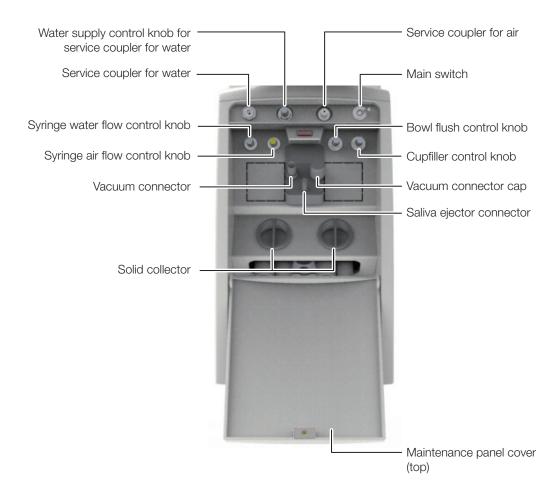


4-3-7 Vac Pac Unit

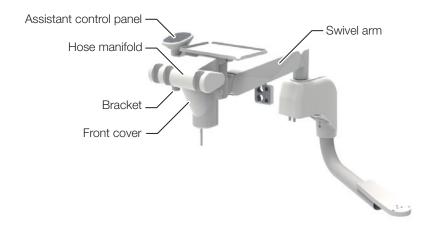


Refer to the Dürr products' instructions for use for operating procedures.


4-3-8 Assistant Unit

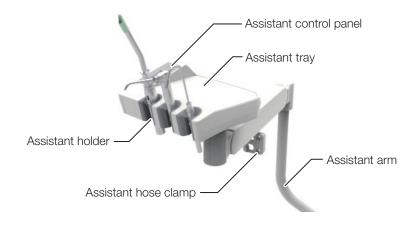

4-3-9 Junction Unit

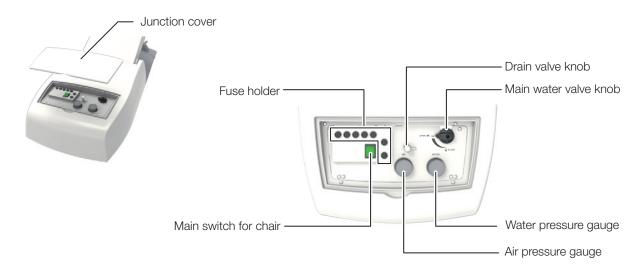

Junction unit (1)



Main water valve knob





The valve is closed.


The valve is open.

5–1 Preparation Before Use

1 Open the main water valve

Press the main switch for chair.

- * When turns on, it will light up.
- (1) Raise the part marked with of the seat as shown in the left figure up to the position that gives some space above the junction unit.
- (2) Remove the junction cover.
- (3) Turn the main water valve knob clockwise to lay it on its side.



2 Turn on the power for chair


Press the main switch for chair.

* When turns on, it will light up.



Operate the main switch for chair by hand.

Cuspidor



Vac Pac

In the case of a Vac Pac unit, the main switch is located under the doctor table.



3 Switch on EURUS.

Turn the main switch to the right (I)

Nothing should be placed on the cupfiller base when the main switch is turned on. Water may not be supplied normally during cupfiller operation.

When turning on the main switch, sensitivity of touch panel will be initialized. Do not turn on the power while touching the panel by fingers.


Turning on the power while touching the panel may lead to the reduction of the sensitivity of the panel.


If the detection is incorrect, turn off the power and wait for approx. 5 seconds. Then, turn on the power again.




Operate the main switch by hand.

Peel off the film attached to the touch panel before initial use. Using the touch panel with the film attached may lead to incorrect operation, resulting in injury.






The program version information differs depending on the month of purchasing (manufacturing) and specifications.





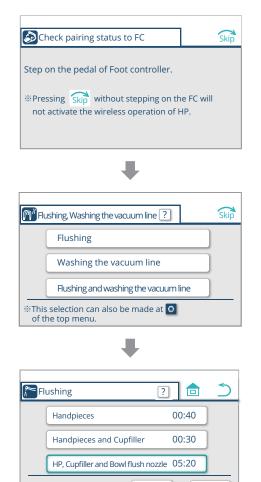

Hold down the pedal of the wireless foot controller until the flushing screen appears.

If it does not happened while holding down the pedal of the foot controller, refer to the "Foot controller (wired/wireless)" [pages 146 to 149].

* The wireless pairing screen does not appear if the foot controller is wired.

Press the 'Flushing' switch.


If the washing function for vacuum line is not equipped, the screen shown in the left figure does not appear. The screen titled "Without washing function for vacuum line" will be displayed.

The flushing screen is displayed.

Perform flushing, referring to "Selection and implementation of flushing method" [pages 171 to 190].

* To cancel the process, press skip.

For Vac Pac unit type




٥

OK

* For Vac Pac unit type, the screen shown in the left figure appears.


Without washing function for vacuum line



Home screen



Once the flushing process is completed, the home screen is displayed. For the description of respective switches and indications, see "Doctor's unit operation panel" [pages 82 to 105].



5 Be sure to respond appropriately if an error occurs

If an error occurs during the startup process, the check mode screen is displayed on the touch panel. See explanation on [pages 260 to 262], and respond appropriately according to the indicated method.

To display the next screen, press the skip switch.

If five or more errors occur, press the skip switch to check errors other than the ones indicated on the first page.

6 Perform startup inspection

- ① Confirm that the discharge of retained water has been completed.
- ② Operate the switches and the foot controller to confirm that the chair and the handpieces/syringes function normally.

(Connect the handpieces/syringes before performing the operation check.)


7 Prepare for the procedure

- 1) Put an cup on the cupfiller base of the cuspidor unit.
- ② Attach the vacuum/saliva ejector tip to the vacuum/saliva ejector handpiece.



Be sure to perform maintenance inspection before use (startup inspection to confirm that the product functions normally).

Operation without performing maintenance inspection may result in injury and damage to peripheral equipment.



5–2 After use

1 Turn off the power for chair


When turned off, the light goes off.



CAUTION

Operate the main switch for chair by hand.

Cuspidor



2 Power off the unit


Push down the main switch to the left side (O).



CAUTION

Operate the main switch by hand.

Vac Pac




3 Close the water main valve

Turn the main water valve knob counterclockwise until the knob is positioned vertically.



CAUTION

To prevent accidental leakage, be sure to close the main water valve at the end of day.



Main water valve knob





The valve is open.

The valve is closed.

5–3 Operating the main switch for chair during treatment (when the main switch for chair is available)

1 Turn off the power for chair

Press the main switch for chair.

When turning off the chair, "E06: Communication with chair" is displayed on the touch panel because of the interruption of communication between unit and chair, then LED indicator of the cuspidor unit lights up in orange, which is not malfunction.

Touch panel



LED indicator



2 Turn on the power for chair

Press the main switch for chair.

Press the main switch for chair when 5 seconds or more have passed after turning off the main switch for chair.


Stick switch for manual operation

The position and/or availability of the stick switch may differ according to the specification selected.

Doctor control panel Membrane switch (Holder)



Switches for manual operation



Assistant operation panel (Vac Pac Unit type)



Switches for manual operation

5–4 Raising/lowering the chair and raising/reclining the backrest (manual operation)

Cart/Swing mount

Stic	k switch	Operation			
Pushing direction	Label indication	panel switch	Operation		
	× 7	(-)	The chair is raised		
	* * * 7 7 * * * * * * * * * * * * * * *	(+) (+)	The chair is lowered		
	↑ ∠ • • • • • • • • • • • • • • • • • • •	N.	The backrest is raised		
	↑ (E) \ _ 7	W.	The backrest is reclined		

^{*}The chair is operated while the stick switch is pushed down or the switch is pressed.




WARNING

Before raising/lowering the chair, confirm that no human body part, limb, or obstacle is obstructing the chair.

Before reclining the backrest, confirm that the patient's arm or hand is not placed between the backrest and the seat.

Before raising the backrest, confirm that the patient's arm or hand is not placed between the backrest and the armrest.

[Reference] Precautions when a patient is seated [page 20]



Foot switch

Stick	switch		
Pushing direction	Label indication	Operation	
	× 7 7	The chair is raised	
	¥ → 77	The chair is lowered	
	↑ ∠ 17) →	The backrest is raised	
	↑ (L) 1 ↓	The backrest is reclined	

^{*} The chair is operated while the foot switch is pushed down.



Before raising/lowering the chair, confirm that no human body part, limb, or obstacle is obstructing the chair.

Before reclining the backrest, confirm that the patient's arm or hand is not placed between the backrest and the seat.

Before raising the backrest, confirm that the patient's arm or hand is not placed between the backrest and the armrest.

[Reference] Precautions when a patient is seated [page 20]

Stick switch for automatic operation

The position and/or availability of the stick switch may differ according to the specification selected.


Doctor control panel Membrane switch (Holder)

Switches for automatic operation



Membrane switch (Rod)

Switches for automatic operation



Assistant operation panel (Assistant Unit type)

P 0 | 1 | 1 | 2 | Stop chair auto motion

Switches for automatic operation

Assistant operation panel (Vac Pac Unit type)



5–5 Moving the chair to the preset position (automatic operation)

Cart/Swing mount

	Stick switch		Operation		
	Pushing direction	Label indication	panel switch	Operation	
I		LP 1 2 0	1	The chair is moved to the preset "Treatment position 1".	
II		1 LP (2)	2	The chair is moved to the preset "Treatment position 2".	
III		1 LP 2	0	The chair is moved to the preset "Entry/exit position". By pushing again after movement completion, the headrest is housed	
	•	NO/	U	in the case of headrest (electrohydraulic).	
		(ĹP)	LP	The chair is moved to the preset "mouth rinsing position".	
IV		1 2		By pushing again after movement completion, the chair is moved to the position prior to the "mouth rinsing position".	


Do not hold down the preset switches (1) or (2), automatic return switch (0), or last position switch (1) for five seconds or longer. If pressed for five seconds or more, a buzzer sound is heard, and the chair position at that point is memorized as the set position.

[Reference] Automatic operation setting [page 168]




WARNING

Before moving the chair, confirm that no human body part, limb, or obstacle is obstructing the chair.



Angle and up/down of headrest



5–6 Operating the headrest (manual type)

Adjustment of the headrest

The headrest (manual type) is capable of flexibly adjusting the inclination of the patient's head for treatment in the upper/lower jaw.

It is also possible to manually extend/fold the headrest in accordance with the patient's height.

Angle adjustment of the headrest

- 1. Insert the operator's hand beneath the headrest to support the patient's head.
- 2. Press in the control lever with the other hand to make the headrest movable.
- 3. Adjust the headrest to an angle that matches the required treatment, and release the control lever to lock the headrest.

Up/down adjustment of the headrest

- 1. To raise the headrest, pull the headrest up slowly while holding it.
- 2. To lower the headrest, apply the operator's hand to the headrest, and pull it down slowly while pressing the headrest lowering button.

Do not apply excessive load or impact to the headrest while it is extended. Do not hit the headrest from above. Otherwise, failure may result.



WARNING

If the backrest is to be moved while the headrest is extended, confirm that there is no object obstructing or coming into contact with the chair. Otherwise, damage or injury may result.

When operating the headrest, be careful not to get the operator's hand or finger caught around the control lever or between the headrest and the backrest.

When adjusting the angle or up/down, be sure to apply the operator's hand to the headrest and support the patient's head. Otherwise, an accident or injury may result.

Be sure that the headrest is not rattling or making abnormal noise. Moving the headrest while rattling may result in an accident or injury.




Headrest (electrohydraulic)



Stick switch for headrest (electrohydraulic)

The position and/or availability of the stick switch may differ according to the specification selected.

Doctor control panel Membrane switch (Holder)

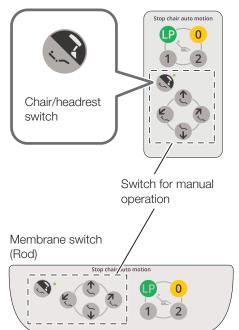

5–7 Operating the headrest (electrohydraulic type)

Cart/Swing mount

For operation with the manual operation switch, press the chair/headrest switch to switch over to the headrest function (the light is turned on).

	k switch	Operation		
Pushing direction	Label indication	panel switch lamp is turned on	Operation	
	× 7		Raise	
	∠ ↑ 7	\	Lower	
		7	Raise	
		N.	Recline	

^{*} The headrest is operated while the stick switch is pushed down or the switch is pressed.

Do not apply excessive load or impact to the headrest while it is extended. Do not hit the headrest from above. Otherwise, failure may result.




Before moving the headrest, confirm that the patient's head is placed in the correct position. Operator must not take their eyes off the patient during movement.

[Reference] Precautions when a patient is seated [page 20]

Do not use the unit at an angle that causes discomfort to the patient.

When moving the headrest, confirm that there is no object obstructing. Be very careful not to get an object or human body part caught between the headrest and the backrest.

When the backrest is reclined while the patient is seated, do not raise or lower the headrest with the patient's head on it.



Foot switch

Stick switch		
Pushing direction	Label indication	Operation
	× 7	Raise
	× 7 7	Lower
		Raise
	(<u>U</u>) 7	Recline

^{*} The chair is operated while the foot switch is pushed down.

Do not apply excessive load or impact to the headrest while it is extended. Do not hit the headrest from above. Otherwise, failure may result.



Before moving the headrest, confirm that the patient's head is placed in the correct position. Operator must not take their eyes off the patient during movement.

[Reference] Precautions when a patient is seated [page 20]

Do not use the unit at an angle that causes discomfort to the patient.

When moving the headrest, confirm that there is no object obstructing. Be very careful not to get an object or human body part caught between the headrest and the backrest.

When the backrest is reclined while the patient is seated, do not raise or lower the headrest with the patient's head on it.

5–8 Turning the armrest

If the armrest hinders entry/exit or treatment, it may be turned backward. Both the left and right armrests can be turned.

(1) Pull the root of the armrest (back side) upward.



(2) Turn the armrest backward while holding it up.

Turning angle: 90 or 135 degrees



(3) To return the armrest to the original position, turn it forward in the same procedure.

The armrest is locked when it comes to the normal position






When turning the armrest, confirm that there is no obstruction. Operator must be careful not to get their hand or finger caught.

Do not move the chair while the armrest has been turned backward. Return the armrest to the normal position before moving the chair.

Handle



Base mount

Moving the doctor table forward/backward and right/left Hold the handle and slowly move the doctor table.



WARNING

Do not apply a load exceeding 3 kg to the doctor table. Otherwise, damage or injury may result.

Height adjustment of the doctor table


The doctor table is adjustable at three heights.

After adjusting, move the doctor table right and left to confirm hat the downward movement of the table is locked.

* The chair lock function will activate when strong force is applied on the top or bottom of the doctor table.



- (1) Remove the adjust bolt.
- (2) Remove the hole plugs (2 places).
- (3) Pull up the first arm.
- (4) Move the lock ring to the desired table height's groove.
- (5) Return the first arm to its previous position.
- (6) Insert the adjust bolt in the hole corresponding with the position of the lock ring.

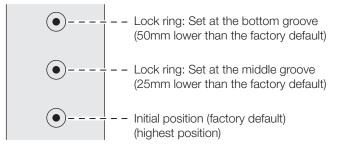


(7) Insert the hole plugs (2 places) in the open holes.



WARNING

When adjusting the table height, confirm that the main switch is turned off. Accidentally pressing the switches or foot pedal will lead to unexpected operation of the product, which may cause injuries.

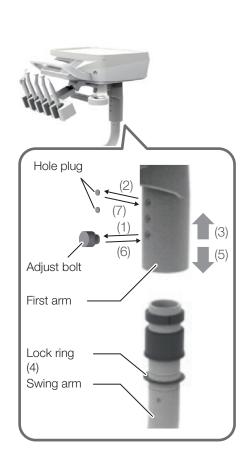



Cart

The height of the doctor table can be adjusted in the range as shown in the left figure.

To change the height, loosen the lock knob and pull up/down the doctor table. After changing the height to the desired position, tighten the lock knob securely.

Loosen the lock knob → turn it counterclockwise

Tighten the lock knob → turn it clockwise

Moving the doctor table upward/downward without loosening the lock knob may cause damage to the product.

Be sure to loosen the lock knob first, then move the doctor table upward/downward.




Swing mount

Height adjustment of the doctor table (Rod)

Balance arm brake release switches are located on the handle.

Grasp the handle and press the balance arm brake release switch to release brake and adjust the table height.

Release the balance arm brake release switch at the desires table position and the balance arm position will be locked.



Height adjustment of the doctor table (Holder)

The height of the doctor table can be adjusted in the range as shown in the left figure.

To change the height, release the brake first by pressing the balance arm brake release switch at the center of the handle. Then, move the doctor table upward/downward.





Moving the doctor table upward/downward without releasing the brake may cause damage to the product.

Be sure to release the brake first by pressing the brake release switch. Then, move the doctor table upward/downward.




5-10 Control of the assistant tray

- (1) Moving the assistant tray forward/backward Hold the assistant tray and slowly move it forward/backward.
- (2) Turning the assistant tray Hold the assistant tray and slowly turn it. It is possible to turn the tray only.

When moving the assistant tray forward/backward, make sure there is nothing on the assistant tray.



Do not apply a load exceeding 1.5 kg to the assistant tray. Otherwise, damage or injury may result.



Height adjustment of the assistant tray

The height of the tray can be adjusted by stopping the arm angle in the range from 0 to 40 degrees (see the figure on the left).

To change the height, move the tray while holding the arm part.

To raise the height

Hold the tray when moving it upward.

To lower the height

First move the arm upward while pressing the unlock button, and subsequently move it downward.

Move the tray to the desired height, and release the unlock button.

When adjusting the height of the assistant tray, make sure there is nothing on the assistant tray.

To lower the height, be sure to press down the unlock button during adjustment. Lowering the height without pressing the unlock button may cause damage to the product



Do not apply a load exceeding 1.5 kg to the assistant tray. Otherwise, damage or injury may result.




(Example of display) Micromotor MX2










5-11 Handpiece

When a handpiece other than the syringe is picked up from the instrument holder, the operation screen for the handpiece is displayed on the touch panel. Subsequently, operate the foot controller to move the unit.

[Reference] Micromotor [pages 116 to 129]
Ultrasonic scaler [pages 130 to 132]
Air Turbine /motor [pages 133 to 135]
Vacuum handpiece [page 152]
Saliva ejector handpiece [page 152]
Foot controller (wired/wireless) [page 146]

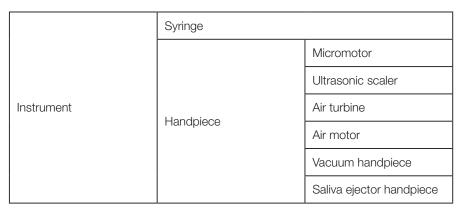

When the handpiece is returned to the instrument holder, the home screen is displayed.

Handpiece priority function (first priority)

Only the handpiece that is picked up first is operable.

If two or more handpieces are picked up from the instrument holder, and if the handpiece picked up first is returned to the holder, a message [C12: HP first priority] is displayed.

This message disappears if all handpieces are returned to the instrument holder.



CAUTION

Repeated actions of picking up and returning the handpiece may cause its hose twisted.

Check the hose periodically to see if it is not twisted. If twisted, unwind it before use.


Continual use of the handpiece with its hose twisted will cause the kinks in the hose or breaking of the wire, making the handpiece unusable.

5–12 Doctor's unit operation panel

Touch panel (home screen)

The overview of indications and switches on the touch panel is as follows.



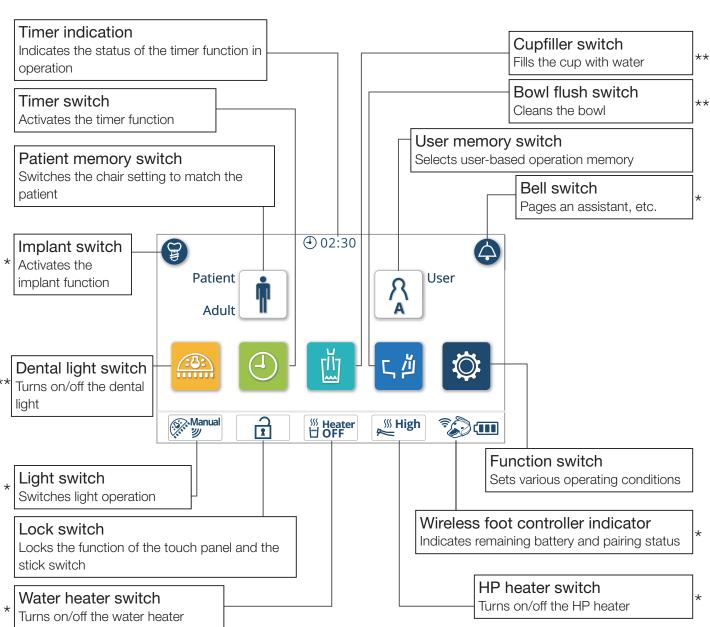


* Not indicated if the function is not installed

^{**} It is displayed in gray if the function is not installed.

Touch panel (handpiece screen)


The overview of indications and switches on the touch panel is as follows.

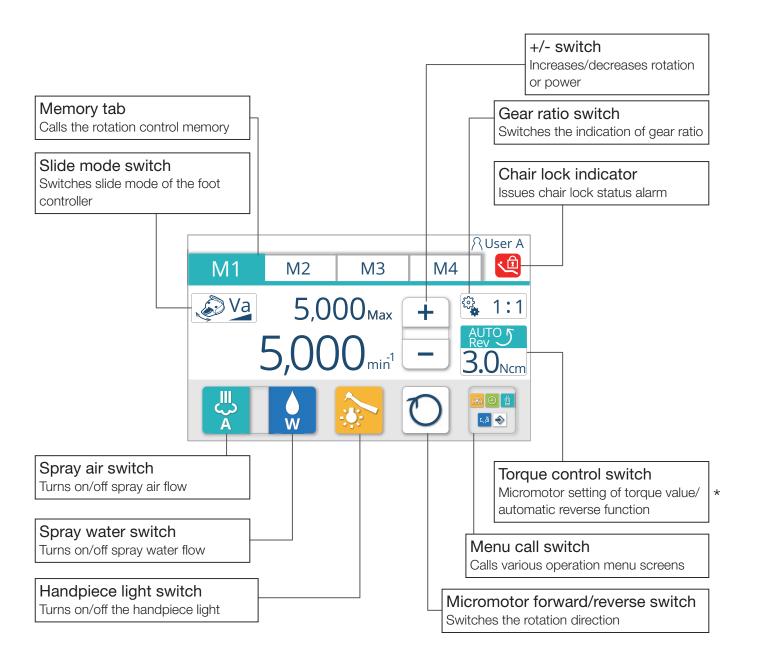

^{*} Not indicated if the function is not installed

Touch panel (Implant screen)

The overview of indications and switches on the touch panel is as follows.

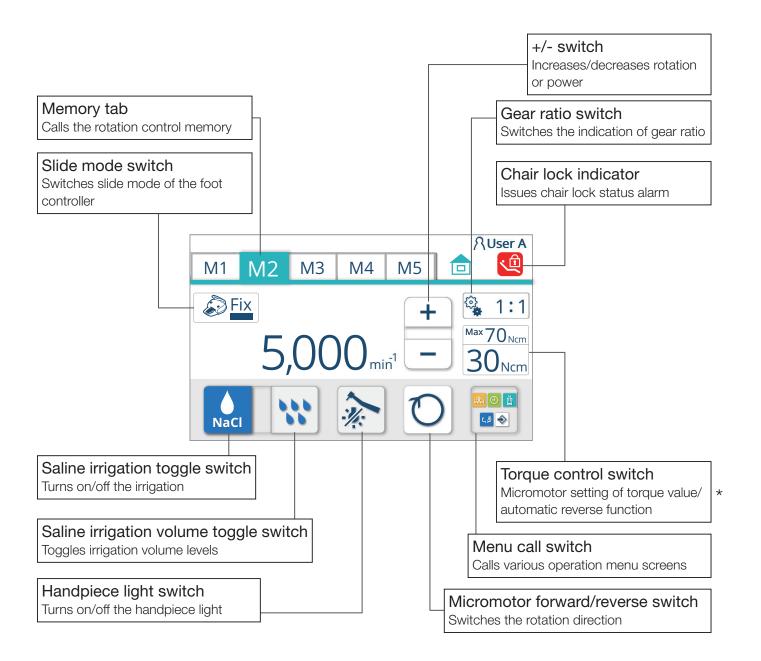


^{*} Not indicated if the function is not installed

Membrane switch

The overview of indications and switches on the operation panel is as follows.



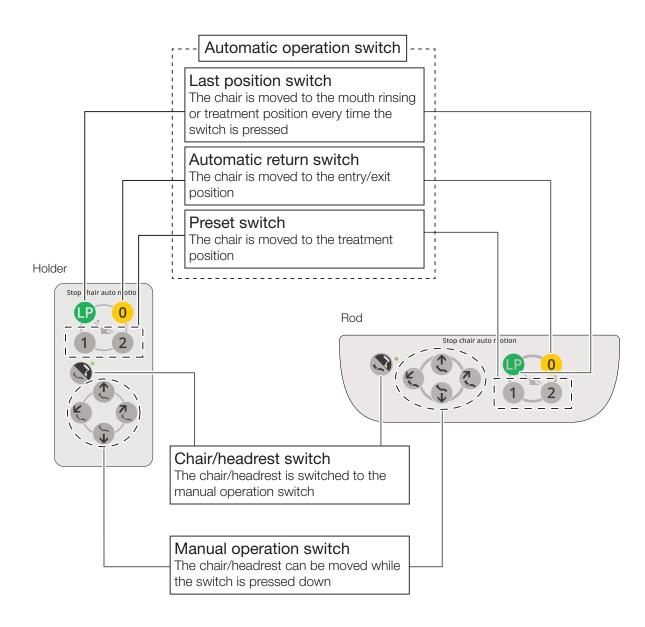



Last position switch

When pressed in the treatment position, the chair is moved to the mouth rinsing position.

When the switch is pressed again, the chair is returned to the treatment position prior to mouth rinsing.



Automatic return switch

The chair is moved to the entry/exit position.

* In the case of headrest (electrohydraulic), by pushing this switch again after the chair comes to the complete stop, the headrest is housed.



Preset switch

When 1 is pressed, the chair is moved to treatment position 1.




When 2 is pressed, the chair is moved to treatment position 2.

Do not hold down the preset switch, automatic return switch, or last position switch for five seconds or longer.

If pressed for five seconds or more, a buzzer sound is heard, and the chair position at that point is memorized as the set position.

[Reference] Automatic operation setting [page 168]



Manual operation switch

Manually operates "Raise/lower" and "Raise/recline" of the chair/headrest.

Switch	Operation
(The chair is raised / The headrest is raised
*	The chair is lowered / The headrest is lowered
K	The backrest is reclined / The headrest is reclined
	The backrest is raised / The headrest is raised

^{*}The chair/headrest can be moved while the switch is pressed down



When the headrest function is selected, the lamp is turned on

Chair/headrest switch


Switches the chair/headrest functions to the manual operation switch. When the headrest function is selected, the lamp is turned on.



Before moving the chair, confirm that no human body part, limb, or obstacle is obstructing the chair.

Take particular precautions for the movement and behavior of children during operation.





Structure of user/patient memories

Up to six user memories (A to F) and up to three patient memories (Adult, Child and Elderly) can be set.

[Adult]

: Adult mode



A recommended mode for an adult patient of a standard figure; In addition to the automatic return switch **0** and the last position switch **P**, the preset switches **1 2** can be set for up to six user memories (A to F).

[Child]

: Child mode



A recommended mode for a child patient or a patient of a small figure;

The automatic return switch 0, the last position switch 1, and the preset switches 1, 2 can be set respectively.

[Elderly]


: Elderly mode




A recommended mode for an elderly patient or a patient who requires special considerations;

The automatic return switch 0, the last position switch 1, and the preset switches 1 2 can be set respectively. The angles of the backrest and legrest can be limited, and other settings are possible.







Calling the Structure of user/patient memories

1.Press the user memory switch ...
The "Selection of user" screen is displayed.

2.On the "Selection of user" screen, press the ? switch. The "Structure for Patient and User" screen is displayed.

Press the a switch to return from the present screen to the home screen.

Press the \supset switch to return from the present screen to the previous screen.

Patient memory selection switch

The treatment position setting of the chair can be switched in accordance with the patient to be treated.

Every time the switch is pressed, the mode is toggled "Adult" > "Elderly" > "Child".




User memory switch

The preset chair position for each user and the initial settings for handpieces upon powering on can be memorized, and selected when necessary.



1. Press the user memory switch . The "Selection of user" screen is displayed.

2. On the "Selection of user" screen, press the memory switch for the user to be called for selection.



Press OK to call the settings for the newly selected user, and return to the home screen.



∧User A






Name registration

A name can be registered for each user memory.

1. Press the user memory switch [].

The "Selection of user" screen is displayed.



 On the "Selection of user" screen, press the switch for the user memory for selection and name registration. (In this example, User memory A is selected.)

Press the name registration switch do view the "Registration of name" screen for the selected user.



3. Enter the name using the keyboard.

Press **OK** to view the "Selection of user" screen.

User name can be entered in alphabetical or numeric format up to nine digits.

When switching alphanumeric input, press the alphanumeric switch 123.

Press the backspace switch to delete the previous (left) character at the cursor position during the character input.


In this example, the name "BELMONT" has been entered. The registered name is indicated for the User memory A box and displayed at the top right.




* The registered name is indicated to the right of the user memory switch on the home screen.

Copying the chair preset

The settings for the chair preset switches 1, 2 in the Adult mode can be copied to another user memory.





2. Select the "Copied from" user from [A] to [F].

The "Copied from" switch indication is changed to show the selected user.



3. Press the "Copied to" switch and select the "Copied to" user from [A] to [F].

The "Copied to" switch indication is changed to show the selected user.

Press the ok switch to view the popup screen for confirmation.




4. To confirm, press ok.

The copying is completed, and the "Selection of user" screen is displayed.


Press x to return to the previous screen without copying.

Copying the handpiece setting

The initial setting of a handpiece upon powering on can be copied to another user memory.



1. On the "Selection of user" screen, press the "Copy of handpiece setting" switch ...



2. Select the "Copied from" user from [A] to [F].


The "Copied from" switch indication is changed to show the selected user.



3. Press the "Copied to" switch and select the "Copied to" user from [A] to [F].

The "Copied to" switch indication is changed to show the selected user.

Press **o**k to view the popup screen for confirmation.



4. To confirm, press ок

The copying is completed, and the "Selection of user" screen is displayed.

Press x to return to the previous screen without copying.



Dental light switch

Turns on/off the dental light;

On/off is toggled;

- * Pressing and holding the switch while the light is on for 2 seconds or more changes the mode into Composite Safe.
- * The ceiling light and the track light are not operable.



Timer switch

For the use and setting of the timer



<How to use the timer>

Time for the timer can be selected from four memories.

1. Press the timer switch

The "Timer" screen is displayed.



2. Select a memory (in this example, "Timer D: 5 minutes" is selected)

The operation/setting screen for Timer D is displayed.

Press the home switch at to cancel the operation and return to the home screen. To return to the previous operation screen, use the return switch.



3. Change the timer setting

: increase the set time

: decrease the set time

Press the store switch to save the changed setting into the memory.



4. Change the alarm volume for the timer

When the alarm volume adjustment switch wis pressed, the "Timer alarm volume adjustment" screen is displayed.

Press the touch bar graph ____ to adjust the alarm volume in five levels.

Press the alarm sound switch | (1) to mute or de-mute the alarm.

Once adjustment is completed, press the **OK** switch to return to the previous screen.




5. Press the start to start the countdown of the timer The subtraction timer is started.



Press the pause to pause the timer operation. To restart the timer, press the start .

Press the stop • to cancel the timer operation, and return to the screen in 3.



6. Once the timer countdown is completed, an alarm sounds Alarm sounds for the specified time, then it stops automatically.

Press the stop to stop the alarm sound, and return to the home screen.

* If the timer operation is performed on the handpiece screen while the handpiece is picked up, the display returns to the relevant handpiece screen.






7. Returning to the home screen during timer operation

Press the home switch while the timer is operating to return to the home screen. The timer operation status is displayed at the top of the screen. When the timer countdown is completed on the home screen, the screen in 6 is displayed.

* With the handpiece being picked up, even if the timer switch is pressed after pressing the menu call switch , the timer will not start, and the display returns to the handpiece screen.






Once the countdown of the timer is completed with the handpiece being picked up, timer switch appears on the screen.

If the timer switch ① is pressed, handpiece display appears on the screen. If the handpiece is returned without pressing the timer switch ②, the display shown in 6 appears.





8. Changing the mode into timer display

Press the timer switch 49 during the countdown process to show the timer display on the screen as shown in 5.



Cupfiller switch

This is a switch for filling the cup, installed separately from the sensor cupfiller. When this switch is pressed, water is released from the cupfiller nozzle. Water is also released from the bowl flush nozzle to flush the cuspidor bowl.

Cupfiller operates by timer for a specified time period.

To stop cupfiller before the specified time is elapsed, press this switch again.

Before using cupfiller, put a cup on the cupfiller base.

Otherwise, the wall and the chair may be spattered with water.

Cupfiller operates for a specified time period, regardless of the water level in the cup. Be careful not to overflow the cup.



Bowl flush switch

Water is released from the bowl flush nozzle to flush the cuspidor bowl (approx. six seconds).


Hold down the switch for two seconds or longer for continuous flushing. Press this switch again to stop flushing.



Function switch

For setting various operating conditions [pages 169-222]





Light switch


Call the "Sensor/Manual switch mode" screen to switch the operation mode for the dental light.

Select an operation mode and press **OK** to change the setting.

Press X to cancel the change and exit.

Indication	Mode	Condition
Manual Manual ** *Sensor	Sensor/switch mode	The light can be turned on/off with the touchless switch of the dental light and with the dental light switch
Manual only	Switch mode	The light can be turned on/off with the dental light switch
ON Keep light ON	ON mode	The dental light is continuously turned on at the maximum illuminance. * The light cannot be turned on/off with the touchless switch of the dental light and with the dental light switch
OFF . Keep light OFF	OFF mode	The dental light is continuously turned off * The light cannot be turned on/off with the touchless switch of the dental light and with the dental light switch







Lock switch


To clean the operation panel or to prevent mischief by child patients, the touch panel, membrane switch or the stick can be locked.

Call the "Lock mode" screen and press OK to lock the operation.

During locking, the locking message screen is displayed on the touch panel.

To cancel the operation lock, press and hold the chair/headrest switch of for approx. one second or more.





Water heater switch





HP heater switch

Call the "Water heater (Handpiece)" screen to set water released from the handpiece to warm water, and to set the temperature of water (two temperatures).

Select the heater mode (High, Low, OFF) and press **ok** to change the setting.

Press X to cancel the change and exit.





Wireless foot controller indication

Indicates the remaining battery and pairing status of the wireless foot controller.

As the battery level declines, the indication changes from • to • After a warning popup screen is displayed, the indication is changed to ... Once the popup is displayed, promptly replace the battery with a new one. [Reference] How to replace batteries [page 148]

Press X to close the popup.

If the wireless foot controller has not been paired,



is displayed, and the foot controller is not usable.

If it is not usable, turn off the main switch and reboot the unit, then perform pairing the wireless foot controller.



Bell switch


An assistant, etc. can be paged by using an externally connected device.



Implant switch

Enables the implant function

Air ON / Water ON (Spray ON)



Air OFF / Water ON



Air ON / Water OFF



Air OFF / Water OFF (Spray OFF)



Spray switch

Turns ON/OFF handpiece spray (water and air).

Pick up a handpiece and press the switch to toggle between ON/OFF of A (Air) and W (Water).

In the case of micromotor / air turbine / air motor, two modes or four modes can be selected depending on the spray mode setting.

When set to two modes, Spray ON/OFF is toggled.

When set to four modes, ON/OFF can be respectively toggled for Air and Water.

Regardless of two or four modes, an ultrasonic scaler can toggle between ON/OFF of W(Water) only.

[Reference] Spray mode setting [page 209]

Light on



Light off



Handpiece light switch

Turns on/off the handpiece light.
The light is toggled between on and off.

[Reference] Setting the light activation timing [page 210]




Saline irrigation toggle switch

Each press of this switch turns on or off the irrigation.

Saline irrigation toggle switch



The foot controller can be used instead. Each step on the switch turns on or off the irrigation.

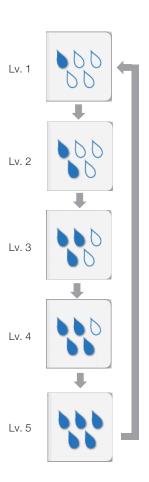

Saline irrigation volume toggle switch

Each press of this switch changes the irrigation volume levels.

The levels can be changed as follows: Lv. 1 \rightarrow Lv. 2 \rightarrow Lv. 3 \rightarrow Lv. 4 \rightarrow Lv. 5 \rightarrow Lv. 1. There are five irrigation volume levels, and the higher the level, the more the irrigation volume.

To turn on or off the volume adjustment, use the saline irrigation toggle switch.

Forward rotation (clockwise)



Reverse rotation (counterclockwise)



Reciprocal mode (unswitchable)



Micromotor forward/



Micromotor forward/reverse switch

Switches the rotation direction of the micromotor.

Forward rotation (clockwise) and reverse rotation (counterclockwise) is toggled. Rotation is set to forward immediately after powering on.

* The rotation direction cannot be switched while the micromotor is being rotated.

(When operating the implant motor)

The foot controller can be used instead.

Each step on the switch toggles the rotation direction (forward/reverse) of the micromotor.





Menu call switch

Calls menu screens for performing the following operations while a handpiece is picked up.

Dental light on/off

[Reference] Dental light switch [page 94]

Use and setting of timer

[Reference] Timer switch [pages 94-96]

Cupfiller

[Reference] Cupfiller switch [page 97]

Cuspidor bowl flush

[Reference] Bowl flush switch [page 97]

Memory of handpiece operating condition setting

[Reference] Store switch (handpiece setting screen) [page 103]





Store switch (handpiece setting screen)

This switch is displayed when the rotation, spray condition and other settings have been changed from the memory on the handpiece screen. Press the switch to overwrite the called memory (M1 to M4) with the changed setting.

Slide mode switch

Switches the slide mode (Va/Fix) of the foot controller. [Reference] Micromotor [page 116]



+/- switch

In the case of micromotor, the maximum rotation value is increased/decreased. [Reference] Micromotor [page 117]



Gear ratio switch

The indication can be switched to rotation that matches the contra angle gear ratio of the micromotor.


[Reference] Micromotor [page 119]

Automatic reverse function and Torque value 3.0 Ncm



Torque control switch

The condition of torque value and automatic reverse function can be set in the case of micromotor that accepts setting in low-speed rotation range. [Reference] Micromotor [pages 121, 122, 124 to 127]



Memory tab

The preset memories of handpiece settings can be called and switched.

The memory tab may not be displayed depending on the handpiece.



[References] Micromotor [page 116]

Ultrasonic scaler [page 130]

Turbine [page 133]

Implant motor [page 136]



Before selection



After selection



Handpiece mode switch

By pressing the switch on the screen for changing the initial flushing time, the setting screen for the "handpiece" flushing time is displayed.

[Reference] Time setting of flushing [pages 181-186]

Before selection



After selection



Cupfiller flushing mode switch

By pressing the switch on the screen for changing the initial flushing time, the setting screen for the "cupfiller flushing" flushing time is displayed.

[Reference] Time setting of flushing (handpiece + cupfiller) [pages 183,184]

Before selection



After selection



Cupfiller, cuspidor bowl flushing mode switch

By pressing the switch on the screen for changing the initial flushing time, the setting screen for the "cupfiller, cuspidor bowl flushing" flushing time is displayed.

[Reference] Time setting of flushing (handpiece + cupfiller + cuspidor bowl) [pages 185,186]



Timer switch for flushing

By pressing the switch on the screen for the flushing setting, the screen for changing the initial flushing time is displayed.

[Reference] Time setting of flushing [pages 181-188]



Store Switch (setting screen for flushing/timer)


By pressing the switch on the setting screen for flushing/timer, time is overwritten by a set time.

[Reference] Timer setting of flushing [pages 181-188] How to use timer [page 94]

5–13 Assistant operation panel

Assistant Unit type



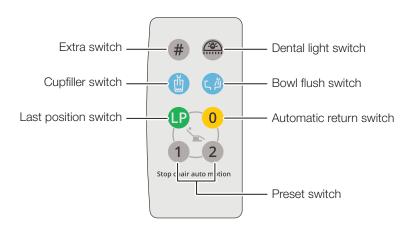



Dental light switch

Turns on/off the dental light;

On/off is toggled;

- * Pressing and holding the switch while the light is on for 2 seconds or more changes the mode into Composite Safe.
- * The ceiling light and the track light are not operable.



Extra switch

When this switch is held down for two seconds or longer, the touchless switch of the dental light is invalidated.

The LED indicator in the cuspidor unit is turned on in pink.

When this switch is held down for two seconds or longer, the dental light sensor is validated.

The LED indicator in the cuspidor unit is returned to the original color.





This is a switch for filling the cup, installed separately from the sensor cupfiller. When this switch is pressed, water is released from the cupfiller nozzle. Water is also released from the bowl flush nozzle to flush the cuspidor bowl.

Cupfiller operates by timer for a specified time period.

To stop cupfiller before the specified time is elapsed, press this switch again.

Before using cupfiller, put a cup on the cupfiller base.

Otherwise, the wall and the chair may be spattered with water.

Cupfiller operates for a specified time period, regardless of water level in the cup. Be careful not to overflow the cup.



Bowl flush switch

Water is released from the bowl flush nozzle to flush the cuspidor bowl (approx. six seconds).

- Hold down the switch for two seconds or longer for ontinuous flushing.
- Press this switch again to stop flushing.



Last position switch

The chair is moved to the gargle position when this switch is pressed in the procedure position.

Press it again to return the chair to the procedure position prior to gargling.



Automatic return switch

The chair is moved to the entry/exit position.

* In the case of headrest (electrohydraulic), by pushing this switch again after the chair comes to a complete stop, the headrest is housed.



Preset switch

When 1 is pressed, the chair is moved to treatment position 1.

When 2 is pressed, the chair is moved to treatment position 2.



Do not hold down the preset switch, automatic return switch, or last position switch for five seconds or longer. If pressed for five seconds or more, a buzzer sound is heard, and the chair position at that point is memorized as the set position.


[Reference] Automatic operation setting [page 168]




Before moving the chair, confirm that no human body part, limb, or obstacle is obstructing the chair.

Take particular precautions for the movement and behavior of children during operation.

Vac Pac Unit type

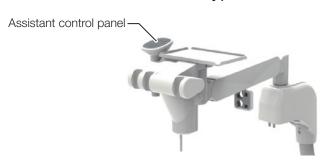

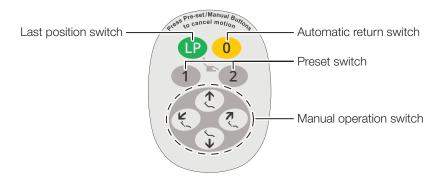









Last position switch

The chair is moved to the gargle position when this switch is pressed in the procedure position.

Press it again to return the chair to the procedure position prior to gargling.

Automatic return switch

The chair is moved to the entry/exit position.

* In the case of headrest (electrohydraulic), by pushing this switch again after the chair comes to a complete stop, the headrest is housed.


Preset switch

When 1 is pressed, the chair is moved to treatment position 1.

When 2 is pressed, the chair is moved to treatment position 2.

Do not hold down the preset switch, automatic return switch, or last position switch for five seconds or longer. If pressed for five seconds or more, a buzzer sound is heard, and the chair position at that point is memorized as the set position.

[Reference] Automatic operation setting [page 168]



Manual operation switch

Manually operates "Raise/lower" and "Raise/recline" of the chair.

Switch	Operation
?	The chair is raised
4	The chair is lowered
K	The backrest is reclined
7	The backrest is raised

^{*}The chair/headrest can be moved while the switch is pressed down



Before moving the chair, confirm that no human body part, limb, or obstacle is obstructing the chair.

Take particular precautions for the movement and behavior of children during operation.

Stick switch

5-14 Cancellation function

To stop the chair movement started by a switch for automatic operation (preset switch, automatic return switch, last position switch, or stick switch for automatic operation), perform one of the following operations.

Stick switch

Operate one of the stick switches (indicated with \bigcirc).



Foot controller

Step on the pedal.



Assistant operation

(Assistant Unit type)

panel

Assistant operation panel

Press one of the switches in the [] frame.



Press one of the switches.

Assistant operation (Vac Pac Unit type)



Doctor control panel Membrane switch (Holder)



Membrane switch

Press one of the switches.

Doctor control panel Membrane switch (Rod)



5-15 Lock function

5-15-1 Chair lock function

When the lock function is activated, indications as listed below are displayed on the touch panel. (When force is applied to the rear link cover, the lock function is activated.)

Home screen



Home screen:



Handpiece screen



Handpiece screen: <a>

When the lock function is activated, the chair movement is stopped, and a popup is opened to notify the abnormality.


Check the popup and promptly eliminate the abnormality.

Eliminate the abnormality or press

to close the popup.

The functions that become locked and the unlocking steps are as follows. [Reference] [pages 112 to 114]

The LED indicator in the cuspidor unit is turned on in orange.

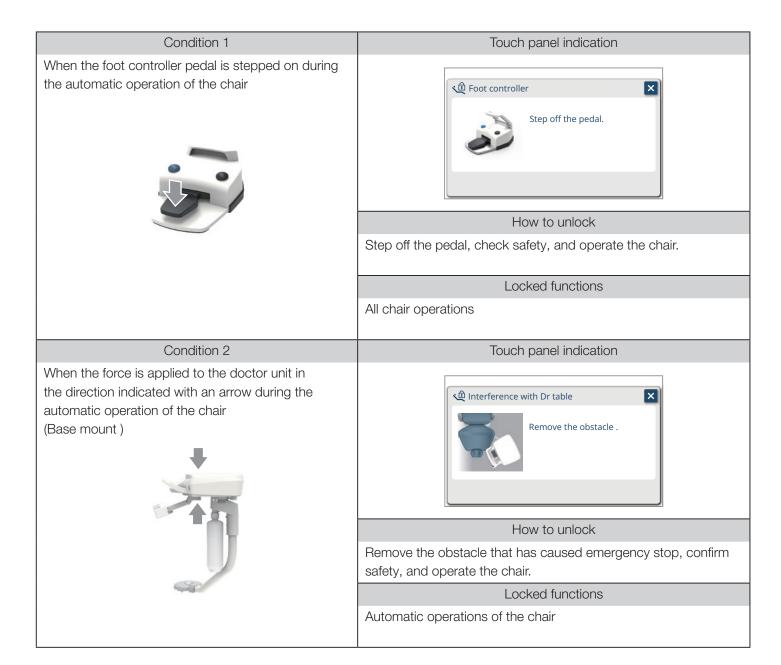

Condition 3

When the doctor arm is rotated to moving area during the automatic operation of the chair (Base mount)



Touch panel indication



How to unlock

Rotate the doctor table until the lock indication on the touch panel disappears.

Locked functions

Automatic operations of the chair

Condition 4

When the force is applied to the assistant arm from the upward/downward direction during the automatic operation of the chair



Touch panel indication



How to unlock

Remove the obstacle that has caused emergency stop, confirm safety, and operate the chair.

Locked functions

Automatic operations of the chair



During the chair movement, force is applied to the rear link cover in the direction indicated with an arrow



Touch panel indication



How to unlock

Remove the obstacle that has caused emergency stop, confirm safety, and operate the chair.


Locked functions

Automatic operations and manual operations of the chair (lowering/reclining the backrest)

5-15-2 Handpiece lock function

When the lock function is activated, indications as listed below are displayed on the touch panel, and the handpiece cannot be used.

The functions that become locked and the unlocking steps are as follows.

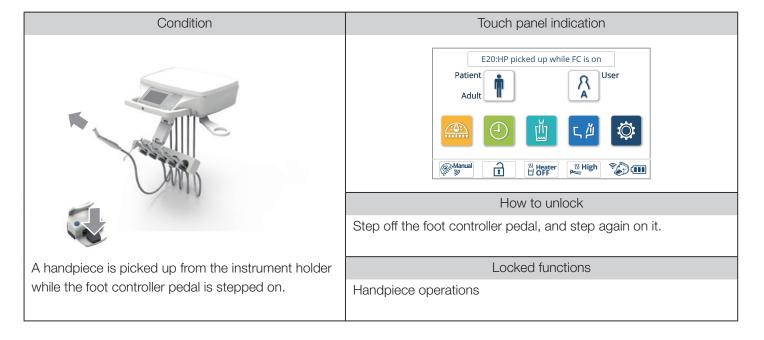

Slide mode (Va/Fix)









5-16 Micromotor

Setting the micromotor slide mode (NBX/NLX plus/NLX nano/MX2/MCX)

When the micromotor is picked up from the instrument holder, the micromotor screen is displayed.

Memory can be selected from four memories (M1 to M4). The memories can be toggled by pressing the memory tab.

The slide mode can be selected from Va and Fix.

Va (Variable)

By setting the maximum rotation, and sliding the foot controller pedal to the left or right, the rotation can be adjusted within the range of the maximum rotation. The rotation is decreased by sliding to the left, and is increased by sliding to the right.

The rotation can be adjusted to the maximum rotation by stepping on the pedal.

Fix (Fixed)

The rotation value can be adjusted up to the setting by the degree of step-in, regardless of the foot controller pedal position.

- 1. Pick up the micromotor from the instrument holder.
- 2. Press the slide mode was to display the slide mode setting screen.
- 3. Select a slide mode.
- 4. Memorize the selection by pressing OK

The micromotor screen is displayed.

Settings of the slide mode are memorized in the starting condition after powering on.

* To cancel the setting change, press x without pressing ok

Maximum rotation M1 M2 M3 M4 S,000 Max + 1:1 5,000 min¹ - 3.0 Ncr Torque value


Automatic reverse function/ Automatic forward function

Setting the maximum rotation (NBX/NLX plus/NLX nano/ MX2/MCX)

- 1. Pick up the micromotor from the instrument holder
- 2. Press the + switch to set the maximum rotation

The setting range of the maximum rotation varies depending on the model of the micromotor (see the figure below).


Automatic reverse function / automatic forward function and torque value are only displayed when setting the low-speed rotation range (NLX plus/MX2).

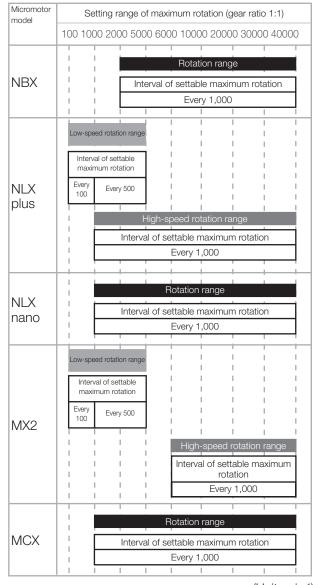

(Unit: min⁻¹)








Memory setting for starting condition after powering on (NBX/NLX plus/NLX nano/MX2/MCX)

When the following setting of handpiece condition is changed, it can be memorized in the steps specified below.

- Maximum rotation
- [Reference] Setting the maximum rotation [page 117]
- Spray condition (ON/OFF/Water/Air) [Reference] Spray switch [page 101]
- Handpiece light condition (ON/OFF) [Reference] Handpiece light switch [page 101]
- 1. Pick up the micromotor from the instrument holder
- 2. Select a memory tab M1 to M4 and press it
- 3. Change the handpiece condition (maximum rotation / spray / handpiece light condition).
- 4. Press the menu call switch ocall the menu screen
- 5. Press the store switch | ◆

The memory setting screen for starting condition is displayed.

- 6. Confirm the displayed setting, and press OK to memorize it.
- * If the OK is not pressed but is pressed, the changed setting is valid until the main switch is turned off, but the setting returns to before the change once the main switch is turned off.







Gear conversion display function (NBX/NLX plus/NLX nano/MX2/MCX)

This function is for indicating a value close to the actual rotation by converting the ratio of contra angle handpiece/ straight handpiece attached to the micromotor. The following four kinds of gear ratio are used for conversion.

- 1:5 (five-fold speed), 1:1 (same speed),
- 4:1 (decelerated to one-quarter speed),
- 16:1 (decelerated to one-sixteenth speed)
- 1. Pick up the micromotor from the instrument holder.
- 2. Select a memory from the tab switch M1 to M4 and press it.
- 3. Press the gear ratio switch 4:1 to display the gear ratio switch setting screen.
- 4. Select a gear ratio.
- 5. Memorize the selection by pressing OK

The micromotor screen is displayed.

Settings of gear ratio are memorized in the starting condition after powering on.

* To cancel the setting change, press x without pressing ok

Overheating prevention function (NBX/NLX plus/MX2/MCX)

Displayed when the overheating prevention function is activated



If the product is used for a long time at a high load, the overheating prevention function is activated and the torque is automatically decreased, in order to prevent the micromotor unit overheating. If this occurs, a buzzer sound is heard, and \checkmark is displayed. While this indication is displayed, the overheating prevention function is activated.

By stopping rotation or using the product at a lower load, the overheating prevention function is deactivated after a certain time has elapsed.



Do not turn off and on again the main switch to deactivate the overheating prevention function. This may cause burn out due to the overheating of the micromotor unit.



For proper use, be sure to carefully read the instructions for use attached to the relevant micromotor in advance.

Slide mode (Va/Fix) Maximum rotation (displayed only in Va mode) Memory tab Gear ratio . Use · A M1 M4 €<u>}</u> 🔊 Va 5,000_{Max} 1:1 + 3.0_{Nc} Ç∄ 🍨 Actual rotation (when the foot controller is on) Rotation in the present foot controller slide position (when the foot controller is off) Torque value Automatic reverse function/

NLX plus

In the case of micromotor NLX plus, if the maximum rotation is set in the low-speed rotation range (100 to 5,000 min-1), the torque value, the applicability of automatic reverse function, and the applicability of automatic forward function can be set.

Automatic reverse is a function that automatically switches to reverse rotation (counterclockwise) when the load exceeds the preset torque value in the low-speed rotation range (0.3-3.0 Ncm).

Automatic forward is a function that automatically switches to reverse rotation (counterclockwise) when the load exceeds the preset torque value in the low-speed rotation range (0.3-3.0 Ncm), and then returns again to forward rotation (clockwise) when the load disappears.



Automatic forward function





Setting of a torque value

- 1. Pick up the micromotor from the instrument holder.
- 2. Select a memory from the tab switch M1 to M4 and press it.
- 3. Press the torque control switch $\frac{1000}{3.000}$ to display the torque setting screen.
- 4. Press the + switch to set to the required torque value.

<Value can be selected from:>

0.3/0.4/0.5/0.6/0.7/0.9/1.0/1.2/1.4/1.8/2.1/2.3/2.7/3.0

When + is pressed, the torque value toggled upward among the options above.

When — is pressed, the torque value is toggled downward among the options above.

5. Memorize the selection by pressing OK ...

The micromotor screen is displayed.

Settings of torque value are memorized in the starting condition after powering on.

* To cancel the setting change, press X without pressing OK

Memory tab ∧User A M1 M2 М3 M4 5,000_{Max} 🔊 Va ٩ 1:1 +3.0_{Nc} a 🕖 👸

Automatic reverse function/ Automatic forward function

function 1. Pick up the micromotor from the instrument holder

- 2. Select a memory from the tab switch M1 to M4 and press it
- 3. Press the torque control switch $\frac{1}{3.0}$ to display the automatic reverse function / automatic forward function setting screen

Setting of automatic reverse function / automatic forward



- 4. Select the required automatic reverse function / automatic forward function setting
 - Rev : Set to "No automatic reverse function"
 - Rev : Set to "Automatic reverse function"
 - คือวา : Set to "Automatic forward function"
- 5. Memorize the selection by pressing The micromotor screen is displayed.

Settings of automatic reverse function and automatic forward function are memorized in the starting condition after powering on.


* To cancel the setting change, press X without pressing





If a reverse screw-shaped file, etc. is attached to NLX plus, be sure to set to "No automatic reverse function", and switch the rotation direction using the forward/reverse switch on the micromotor.

If that unit is set to "Automatic reverse function / automatic forward function", the file may get damaged, resulting in injury.

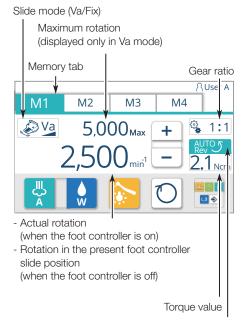

Automatic reverse function/ Automatic forward function

MX2

In the case of micromotor MX2, if the maximum rotation is set in the low-speed rotation range (100 to 5000 min-1), the torque value, the applicability of automatic reverse function, the applicability of automatic forward function, and the time of automatic forward function duration can be set. The applicability of reciprocal mode can be set.

Automatic reverse is a function that automatically switches to reverse rotation (counterclockwise) when the load exceeds the preset torque value in the low-speed rotation range (0.4-3.5 Ncm).

Automatic forward is a function that automatically switches to reverse rotation (counterclockwise) when the load exceeds the preset torque value in the low-speed rotation range (0.4-3.5 Ncm), and then returns again to forward rotation (clockwise) after the specified time of duration (automatic forward duration).



In reciprocal mode, the micromotor oscillates at preset angle, acceleration speed, and torque value.

This mode allows start or stop operation only.

*Rotation speed cannot be adjusted.

When stepping on the foot switch, Fix is displayed as shown in the left figure. When not stepping on the foot controller, Fix is displayed.

Setting of A at the bottom of the screen cannot be changed.


To use the reciprocal mode, designated contra-angle and files are necessary.

Designated contra-angle is shown below: CA ENDO (REF 1600955) by Bien Air

Designated files are shown below: WaveOne® Gold by Dentsply Maillefer

RECIPROC® by VDW







Setting of a torque value

- 1. Pick up the micromotor from the instrument holder
- 2. Select a memory from the tab switch M1 to M4 and press it
- 3. Press the torque control switch 2.1 km to display the torque setting screen
- 4. Press the + switch to set to the required torque value <Value can be selected from:>

0.4/0.7/1.1/1.4/1.8/2.1/2.5/2.8/3.2/3.5

When the + switch is pressed, the torque value toggled upward among the options above.

When the — switch is pressed, the torque value is toggled downward among the options above.

- 5. Memorize the selection by pressing OK The micromotor screen is displayed.
- * To cancel the setting change, press X without pressing OK

Memory tab ∧ User A M2 М3 M4 M1 **₽** Va **4** 1:1 5,000_{Max} +2.1 Nc Ç# 🔷


Automatic reverse function/ Automatic forward function

Setting of automatic reverse function / automatic forward function

- 1. Pick up the micromotor from the instrument holder
- 2. Select a memory from the tab switch M1 to M4 and press it
- 3. Press the torque control switch 2.1 km to display the automatic reverse function / automatic forward function setting screen







- [REV]: Set to "No automatic reverse function"
- Rev : Set to "Automatic reverse function"
- িশ্রেড্রা: Set to "Automatic forward function"
- Reciprocal mode": Set to "Reciprocal mode"

[Reference] Setting the reciprocal mode [pages 127 to 129]

OK



c,∌

5. Memorize the selection by pressing

The micromotor screen is displayed.

Settings of automatic reverse function, automatic forward function, and reciprocal mode are memorized in the starting condition after powering on.

* To cancel the setting change, press x without pressing



If a reverse screw-shaped file, etc. is attached to MX2, be sure to set to "No automatic reverse function", and switch the rotation direction using the forward/ reverse switch on the micromotor.

If that unit is set to "Automatic reverse function / automatic forward function", the file may get damaged, resulting in injury.

Memory tab M1 M2 M3 M4 S,000 Max + 1:1 2,500 min - 2.1 Ncr

Automatic reverse function/ Automatic forward function

Setting of automatic forward function duration

- 1. Pick up the micromotor from the instrument holder
- 2. Select a memory from the tab switch M1 to M4 and press it
- 3. Press the torque control switch 2.1 to display the automatic reverse function screen






- 4. Select automatic forward function from the automatic reverse function / automatic forward function setting
- 5. Press the + switch to select from 0.0-25.4 seconds
 The selection can be made at an interval of 0.1 second.
 If pressing and holding the + switch, the time interval is 0.5 second.
- The micromotor screen is displayed. Settings of automatic forward duration are memorized in the starting condition after powering on.

* To cancel the setting change, press X without pressing OK

6. Memorize the selection by pressing

Setting the reciprocal mode Startup setting

- 1. Pick up the micromotor from the instrument holder
- 2. Set the rotation speed at 5000 min-1 or less by pressing +
- 3. Press the torque control switch 3.0 km






4. Press the reciprocal switch Reciprocal mode

When the reciprocal switch is selected, the frame color of it turns blue.

- * Reciprocal mode switch is not displayed when the setting language is Japanese, or the micromotor except MX2 is used.
- * Pressing X switch returns the display to the micromotor screen.





Depending on the situation, the micromotor screen (reciprocal mode) will be displayed right away or a screen that prompts to acquire a license may be displayed.

When the screen that prompts to acquire a license appears

- * Steps 6. to 9. are performed only during the initial setup. Once the setup is complete, the micromotor screen (reciprocal mode) will be displayed right away.
- * Pressing \supset switch returns the display to the torque setting screen.



The screen for entering activation code is displayed.

7. Obtain the activation code from the following website [Reference] How to obtain the activation code [page 129] https://dental.bienair.com/waveone/

When obtaining the activation code, ID code shown at the top-left of screen is necessary.

8. Enter the activation code obtained in Procedure 7.




9. After entering the code, press OK switch



Micromotor screen (reciprocal mode)



A buzzer sounds, and the micromotor screen (reciprocal mode) appears. Setting of the reciprocal mode is memorized in the starting condition after powering on.




If the activation code is incorrect, the screen shown in the left is displayed. After pressing the switch, resume the setting from Procedure 8.

Micromotor screen (reciprocal mode)



Canceling the reciprocal mode

- 1. Pick up the micromotor from the instrument holder The micromotor screen (reciprocal mode) appears.
- 2. Press the Reciprocal switch.



- 3. Press one of the following switches, AUTO, or AUTO, or AUTO, when the switch is selected, the frame color of it turns blue.
- * Pressing X switch returns the display to the micromotor screen.





4. Press OK switch
Micromotor screen is displayed.


Website for obtaining activation code



How to obtain the activation code

Select the "Dental unit" shown in the left figure.

Screen for entering information

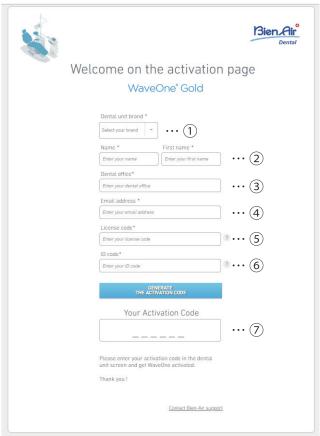

- 1. Enter the following information into the box 1 to 6.
 - 1 Select "Belmont"
 - 2 Enter your name
 - 3 Enter your address
 - 4 Enter your email address
 - 5 Enter the license code contained in the box of contra-angle.
 - 6 Enter the ID code displayed on the touch panel of the doctor unit

[Reference] Setting the reciprocal mode— Startup setting—7. [page 127]

2. Enter the information into the box 1 to 6 and



Activation code will be displayed in the box 7.

Enter the obtained activation code into the box when prompted in Procedure 8—

Startup setting—Setting the reciprocal mode [page 127].

The content of display is subject to change without notice.

Slide mode (Fix/Va) Mode tab Output ∧User A Scaling Perio Endo 🔊 <u>Fix</u> ÇA 🔷


Touch bar graph

∧User A Perio Endo Scaling 🔊 Va 8_{Max}


Maximum output (displayed only in Va mode)

(I) **L**∌ ◆

(Example of indication)







5-17 Ultrasonic scaler

Perio/Endo/Scaling switch setting

When the ultrasonic scaler is picked up from the instrument holder, the electric scaler screen is displayed, and the mode is displayed at the top left.

The mode can be selected from "Perio", "Endo", and "Scaling".

The mode is toggled by pressing the mode tab.

* When using NO PAIN, the mode cannot be selected.

The slide mode can be selected from Fix or Va.

* We recommend selecting "Fix."

Fix (Fixed)

The output is fixed only with the set value.

- 1. Pick up the ultrasonic scaler from the instrument holder
- 2. Press the slide mode switch was to display the slide mode setting screen
- 3. Select a slide mode
- 4. Memorize the selection by pressing

The electric scaler screen is displayed.

Settings of the slide mode are memorized in the starting condition after powering

* To cancel the setting change, press X without pressing

Va (Variable)

By sliding the foot controller pedal to the left or right, the output can be adjusted within the range of the maximum output.


The output is decreased by sliding to the left, and is increased by sliding to the right.

The touch bar graph and output indication are displayed in accordance with the pedal slide position.

The maximum output setting can be changed using the touch bar graph

Output of the electric scaler cannot be changed when the scaler is in operation. After turning off the scaler, change the output by using the touch bar graph


Slide mode Va



Setting of the maximum output in the slide mode Va

- 1. Pick up the ultrasonic scaler from the instrument holder
- 2. Press the touch bar graph that corresponds to the required maximum output value, and select the maximum output between 1 and 10

Slide mode Fix



Setting of the maximum output in the slide mode Fix

- 1. Pick up the ultrasonic scaler from the instrument holder
- 2. Press the touch bar graph that corresponds to the desired output value to select output between 1 and 10 or between 0 and 10. (Output 0 is only selectable when NSK VARIOS VS170 SCALER or NSK VARIOS VS170 LUX SCALER is used.)
- * When the output is 0, the scaler does not vibrate.

 Set it to 0 when you want to use the scaler for irrigation only.

(Example) When the output is 1



To set the output to 0

With the output set to 1, press the touch bar graph . The output will be set to 0.





When using the chip other than the water supply OFF specification, use the scaler with water supply ON (water flowing).

For proper use, be sure to carefully read the instructions for use attached to the relevant scaler in advance.

Perio


🔊 Va

Memory setting for starting condition after powering on

When the following setting of handpiece condition is changed, it can be memorized in the steps specified below.

- Maximum output [Reference] Setting of the maximum output [page 131]
- Spray condition (Water ON/OFF) [Reference] Spray switch [page 101]
- Handpiece light condition (ON/OFF) [Reference] Handpiece light switch [page 101]
- 1. Pick up the ultrasonic scaler from the instrument holder
- 2. Select a mode from the mode tab and press it
- 3. Change the handpiece condition (maximum rotation / spray / handpiece light condition).
- 4. Press the menu call switch to call the menu screen
- 5. Press the store switch

 The memory setting screen for starting condition is displayed.



Endo

∧ User A


a 🕘 💆

Cğ 🔷

Scaling

8_{Max}

- 6. Confirm the setting to be recorded, and press OK to memorize it.
- * If OK is not pressed but is pressed, the changed setting is valid until the main switch is turned off, but the setting returns to before the change once the main switch is turned off.





When using the chip other than the water supply OFF specification, use the scaler with water supply ON (water flowing).

For proper use, be sure to carefully read the instructions for use attached to the relevant scaler in advance.


Touch bar graph (Upper limit output)

(Example of indication) Maximum output: 10 / Operating output: 5 M1 M2 M3 M4 Waser A M1 M2 M3 M4 Waser A I D Max I that match the number of the maximum output are displayed

that match the number of the output level are displayed







5-18 Air turbine/motor

Setting of the slide mode

The initial setting of a handpiece upon powering on can be copied to another user memory.

When the air turbine/motor is picked up from the instrument holder, the turbine screen is displayed.

Memory can be selected from four memories (M1 to M4). The memory number can be switched by pressing the memory tab.

The slide mode can be selected either Va or Fix.

The memory of the air turbine/motor cannot be set individually for Va and Fix. The Va and Fix setting must be common among M1 through M4.

Va (Variable)

Set the maximum output as explained in [page 134].

In operation, the output can be adjusted within the range of this maximum output by sliding the foot control pedal to left (to decrease) or right (to increase) or by depressing (to increase) or releasing (to decrease) the pedal.


Fix


Set the maximum output as explained in [page 134].

The upper limit output can be adjusted to the maximum output value by depressing the pedal regardless of the position of the pedal for the foot controller.

- 1. Pick up the air turbine/motor from the instrument holder
- 2. Press the slide mode switch was to display the slide mode setting screen
- 3. Select a slide mode
- 4. Memorize the selection by pressing OK The turbine screen is displayed.
- * To cancel the setting change, press 🔀 without pressing 🔼 OK

(Example of indication) Maximum output: Change from 8 to 10





Setting of the maximum output

- 1. Pick up the air turbine/motor from the instrument holder
- 2. Press the touch bar graph that corresponds to the required maximum output value, and select the maximum output between 1 and 10

M1

🔊 Va

M2

M3

8

Max

Memory setting for starting condition after powering on

When the following setting of handpiece condition is changed, it can be memorized in the steps specified below.

- Maximum output
 [Reference] Setting of the maximum output [page 134]
- Spray condition (ON/OFF/Water/Air) [Reference] Spray switch [page 101]
- Handpiece light condition (ON/OFF)
 [Reference] Handpiece light switch [page 101]





- 3. Change the handpiece condition (maximum output / spray / handpiece light condition)
- 4. Press the menu call switch to call the menu screen






R User A

ු ව 👩

Ç₿


M4

- 6. Confirm the displayed setting, and press OK to memorize it
- * If OK is not pressed but is pressed, the changed setting is valid until the main switch is turned off, but the setting returns to before the change once the main switch is turned off.





For proper use, be sure to carefully read the instructions for use attached to the relevant air turbine/motor in advance.

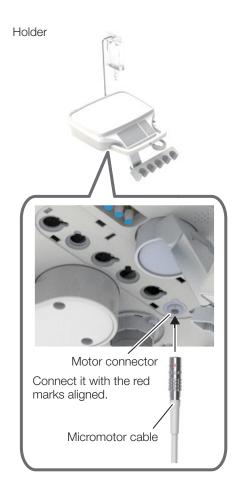


5-19 Implant motor


5-19-1 Connection method

1. Connect the MX-i LED 3rd Gen. micromotor cable to the motor connector.

Make sure that the plug is correctly oriented.

* Connect it with the red marks aligned.

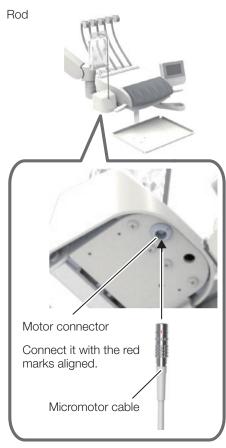



2. Insert the irrigation stand into the hole on the back of the pump cover.

The stand is used to hang a saline bottle.






3. Check that the irrigation line is not expired or damaged.



Use Bien-Air's genuine irrigation lines. They are sterile and disposable. Do not reuse them.



4. Take a disposable irrigation line out of the bag.

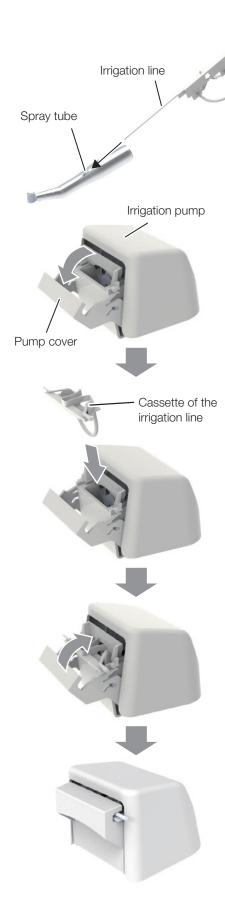

5. Connect the irrigation line to the spray tube of a handpiece (straight or contra-angle).

6. Open the pump cover. Attach the cassette of the irrigation line to the irrigation pump.

Make sure the cassette has been properly clipped.

7. Close the pump cover.


If there is resistance when you are closing the cover, reopen it and check that the cassette is correctly positioned.

When the cover is closed appropriately, it clicks.



When the cover is open or no irrigation line is connected, do not operate the pump. When opening or closing the pump cover, be careful not to pinch your fingers.




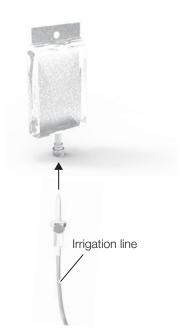


8. Remove the protective cap from the irrigation line. Then insert the tip of the irrigation line into the saline bottle.



If the saline bottle is empty, it cannot automatically be detected by the equipment. Before operation, check the remaining saline level.





9. With the retainer, secure the irrigation line onto the micromotor cable.



5-19-2 Operation method

1. Press the implant switch.

The implant memories screen appears.



2. Select an implant memory.

The implant screen appears.



3. Select a memory.

You can choose from five memories, from M1 to M5. Select the tab that corresponds to the memory you want to choose.

The foot controller (with joystick switches) can be used instead. [Reference] Page 56

Each step on the foot switch changes the selected memory as follows: M1 \rightarrow M2 \rightarrow M3 \rightarrow M4 \rightarrow M5 \rightarrow M1.

When it changes from M5 to M1, the operation sound will change to let you know that the switching cycle has completed.

(If you choose M2)



Pressing the switch returns you to the home screen.



Pressing the implant switch again displays the tab of the memory number that was displayed on the implant screen when you closed the screen.

M1 M2

Fix

M3 M4 M5

5–19–3 Setting handpiece conditions

You can set them with the switches shown below.

Setting the slide mode

Slide mode can only be set to Fix.

Fix

∧User A

20:1 Max 70_{Ncm}

 30_{Ncm}

0

<u>,</u>

In this mode, you can adjust the rotation speed up to the set speed by depressing the pedal regardless of whether the pedal is to the right or left.



For proper use, be sure to carefully read the instructions for use that come with the micromotor in advance.

(Example of indication) If it is changed to 100 min⁻¹



Setting the maximum output

1. Press the "+" or "-" switch.

With these switches, you can increase or decrease the maximum rotation speed.

Between 2,000 and 250 min⁻¹: in increments of 50 min⁻¹

Between 250 and 50 min⁻¹: in increments of 25 min⁻¹

Between 50 and 5 min⁻¹: in increments of 5 min⁻¹

(When the gear ratio is set to 20:1)

When the handpiece is in operation, the actual rotation speed is displayed. When it is not in operation, the set maximum rotation speed is displayed.



Setting the torque value

- 1. Press the torque control switch.
- 2. From among M1 to M5, select the tab that corresponds to the memory of which you want to configure the settings.
- 3. Press the torque control switch $\frac{Max 70_{Ncm}}{30_{Ncm}}$ to display the torque value setting screen.
- 4. Press the + or switch to set the torque to the desired value.

The torque value is displayed and can be set only when it is less than 100 min-1 and the gear ratio is 20:1.

<Selectable values>

Between 10 and 70 Ncm in increments of 5 Ncm

10, 15, 20, 25, 30, 35, 40, 45, 50, 55, 60, 65, or 70

Pressing the + switch increases the torque value in the increments above.

Pressing the - switch decreases the torque value in the increments above.

5. Press the ok switch to save the change.

The implant screen appears.

^{*} If you cancel the change to the setting, do not press the ok switch.

Setting default power-on memories

If you change any of the following handpiece condition settings, you can save the changes by following the steps below:

- Maximum output [Reference] Setting the maximum output [page 141]
- Torque value [Reference] Setting the torque value [page 142]
- Saline irrigation status (ON or OFF)
 [Reference] Saline irrigation toggle switch [page 102]
- Saline irrigation volume [Reference] Saline irrigation volume toggle switch [page 102]
- Handpiece light status (ON or OFF)
 [Reference] Handpiece light switch [page 101]




- 1. From among M1 to M5, select the tab that corresponds to the memory of which you want to configure the settings.
- 2. Change the handpiece conditions (the maximum output, saline irrigation status, saline irrigation volume, and/or handpiece light status) as required.
- 3. Press the "Show the menu" switch to display the menu screen.



4. Press the "Save" switch

→.


The default memory settings screen appears.



- 5. Confirm the displayed content and press [ok] to save it.
- * If you do not press the OK switch and press the Switch instead, the changes will remain effective until you turn off the main switch, but turning it off will discard the changes and restore the previous settings.



For proper use, be sure to carefully read the instructions for use that come with the micromotor in advance.







Gear conversion display function

This function converts the gear ratio of the contra-angle/straight handpiece attached to the micromotor and displays a value that approximates the actual rotation speed.

The following two gear ratios are converted to each other:

- 1:1 (constant speed)
- 20:1 (1/20 deceleration)
- 1. From among M1 to M5, select the tab that corresponds to the memory of which you want to configure the settings.
- 2. Press the gear ratio change switch 4:1 to display the gear ratio change screen.
- 3. Select the desired gear ratio.
- 4. Press the ok switch to save the change.

The implant screen appears.

The gear ratio change setting is saved as part of the default power-on settings.

* If you do not save the change to the setting, do not press the ok switch.

5-20 Syringes

BT14 3WAY syringe SYR-20 3WAY syringe 77-type 3WAY syringe

LUZZANI 6WAY syringe (Minilight) LUZZANI 3WAY syringe (Minilight) LUZZANI 3WAY syringe (Minimate)

DCI 3439 3WAY syringe DCI 3459 3WAY syringe



CAUTION

For proper use, be sure to carefully read the instructions for use attached to the relevant syringe in advance.

Operating BT14 3WAY syringe / SYR-20 3WAY syringe / 77-type 3WAY syringe

(1) Spraying water / air

Press W lever/water button to have water come out.

Press A lever/air button to have air come out.

Press both levers/buttons simultaneously to have spray come out.

Water comes out from the center of the tip, and air comes out from the circumference of the tip.

(2) Rotation of the nozzle


Nozzle rotates through 360°.

If the air is provided immediately after the usage of water or attaching the nozzle, a little water remaining in the nozzle may come out. When providing air, press the A lever/air button for two or three times to confirm that water does not come out.


BT14 3WAY syringe




SYR-20 3WAY syringe



77-type 3WAY syringe



Tip of the nozzle (Common to all types)



5 Operation

TYPE: ES (wired)



TYPE: ESF (wireless)



Carrier Chip air switch Decrease (Stepping) Increase Decrease (Slide) Increase

Type 1

Type 2



5-21 Foot controller (wired/wireless)

Pedal

<When using the micromotor>

The rotation and output can be adjusted by the levels of pedal sliding and stepping.

(Within the range of the indicated maximum rotation)

In Va mode, the rotation is decreased by sliding the pedal to the left, and is increased by sliding it to the right.

<When using the air turbine/motor>

Operation is only possible at a maximum output of 10 max, and on/off operation can be performed by stepping. It is not possible to adjust the output by the levels of sliding/stepping.

<When using the ultrasonic scaler>

The operation is turned on by stepping on the pedal.

It is not possible to adjust the output by the levels of sliding during the operation.

* Output of the electric scaler cannot be changed when the scaler is in operation. After turning off the scaler, change the output, then activate the scaler again.

The output can be adjusted by the level of pedal sliding.

It is not possible to adjust the output by the level of stepping.

(Within the range of indicated maximum output)

The present output is decreased by sliding the pedal to the left, and is increased by sliding it to the right.

Water on/off switch

The spray mode can be switched.

Chip air switch

Air is discharged from the chip of the micromotor or air turbine/motor.

Type 1

The foot controller can be moved by hanging it over the foot.

Type 2

The foot controller can be moved by hand.

The batteries are not included. Insert the batteries referring to "How to replace batteries of the wireless foot controller" [page148].


CONTIO

controller


On the wireless foot controller and on the side of the cuspidor unit, stickers indicating the pairing identification code are attached.

5–21–1 Confirmation of the pairing of the wireless foot

Confirm that the same pairing identification code is indicated.

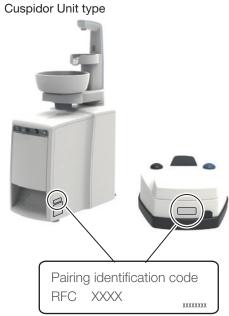

Vac Pac Unit type

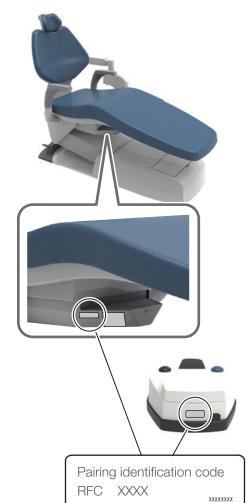

On the wireless foot controller and on the under part of the seat, stickers indicating the pairing identification code are attached.

Confirm that the same pairing identification code is indicated.

Operate the wireless foot controller within one meter of the product.



If more than one unit of the product is used on the same floor, be careful not to operate a wireless foot controller that is paired with another unit.



5-21-2 How to replace batteries of the wireless foot controller When the battery level indication on the home screen becomes , promptly

replace the batteries with new ones.

1. Turn off the main switch



2. Remove the covers of the two battery boxes on the back of the wireless foot controller




Turn off the main switch when replacing batteries.


Otherwise, switches or a pedal is accidentally pressed resulting in unintentional movement, leading to any damage or injury, or the product may not operate normally.



3. Insert two new/charged AA batteries into each box. Use alkali dry batteries or NiMH batteries.



4. Attach the cover of each battery box in order indicated with arrows (1, 2).



A CAUTION

Do not use batteries other than the specified types. Do not mix new batteries with old ones, or mix different types of batteries (e.g. alkali dry batteries with NiMH batteries). Note that improper use of batteries causes leakage or rupture.

Take out batteries if the unit is not to be used for one week or longer.

5 Operation


Connection point


There is a connection point where the rubber cap is removed.



Wireless foot controller







5-21-3 Cable connection of a wireless foot controller

If the wireless foot controller does not operate normally even after replacing the batteries, the unit can be used by connecting the cable contained in the package.

Electric wave used for the wireless foot controller could be interrupted depending on the conditions where the product is used, which might affect the functions of the handpiece. This is not the malfunction of the product.

Be sure to turn off the main switch before connecting the cable. Otherwise, the unit may fail to operate normally.

Before using the cable, take batteries out of the battery boxes. Otherwise, the unit may fail to operate normally.

When removing the cable, be sure to hold the indicated part while pulling it out. Otherwise, disconnection may result.

Cable connection is only for temporary use, and must not be used permanently.

How to connect

When connecting the cable to the chair or cuspidor unit, remove the rubber cap, and insert the connector until it clicks, with the arrow mark facing upward.


The same applies when connecting the cable to the wireless foot controller side.

* Keep the rubber cap of the wireless foot controller to avoid losing it.

How to remove

When removing the cable, be sure to hold the part indicated in the figure while pulling it out, and then attach the rubber cap.

Be sure to attach the rubber cap before using the unit. Use without attaching the rubber cap allows the entry of dust and water, resulting in failure.



5–21–4 Operating precautions for the wireless foot controller

Radio-frequency interference with this product.

This product contains radio equipment that uses the full 2.4 GHz band ((1)), and interference with the mobile identifier band ((4)) is unavoidable. The FSK system ((2)) is employed as a modulation method, and the assumed interference distance is 10 meters ((3)).

The assumed interference distance means the distance at which radio-frequency interference on premises radio stations or specified low power radio stations is anticipated.

Many other devices, including those described below, use the same frequency band as this product: Industrial devices such as microwave ovens, scientific and medical devices, premises radio stations for mobile object identification used for production lines in plants (radio stations that require a license), specified low-power radio stations (radio stations that require no license), and amateur radio stations (radio stations that require a license).

- Check that no premise radio stations for mobile object identification or specified low-power radio stations are operating in the vicinity before starting to use this product.
- 2) If you notice that this product causes hazardous radio-frequency interference on a premises radio station for mobile object identification, promptly stop all emissions of radio waves and contact your local authorized Belmont dealer.
- 3) If you encounter problems such as a case in which this product causes hazardous radio-frequency interference on a specified low-power radio station for mobile object identification, contact your local authorized Belmont dealer.

Devices listed below may cause radio-frequency interference in the 2.4-GHz band:

- Wireless LAN devices
- Receipt computer (used in the hospital wireless environment), mouse, keyboard (Bluetooth, 2.4-GHz band), microscope, intraoral camera, panoramic X-ray equipment, CT, etc.
- Mobile object identification apparatus (such as antitheft devices, entry and exit monitoring systems, etc.)
- Others (such as cautery knives, microwave ovens, etc.)

Certification of equipment

Wireless instruments built into this product are certified as radio-frequency devices for low-power communications in accordance with the Radio Act. Certificates are indicated on the radio-frequency equipment. Therefore, no license is required to use this product. If you take any of the actions listed below with this product, however, you may violate the law and be punished.

- Disassembling or modifying the radio-frequency instruments built into this product
- Removing the certificate labels from the radio-frequency instruments built into this product

Specifications of the wireless foot controller


Transmission system: F1D (FSK)
Maximum transmission power: 1 mW

Battery: 4 × AA batteries

(Alkaline battery or NiMH (rechargeable) battery)

Battery life: Approx. 1,640 hours - Using AA Eneloop batteries


- Used at practices for 15 to 20 patients per day
- Used 5 days per week, one of which it is used only in the morning
- * The battery life varies according to the use environment (frequency of use, radio quality, etc.).
- * Eneloop is a registered trademark of the Panasonic Group.



5-22 Maintenance panel

- (1) Service coupler for water Used to supply water to external devices.
- (2) Water supply control knob for (1) service coupler for water.

 Used to adjust the amount of water supplied for (1) service coupler for water.
- (3) Service coupler for air
 Used to supply air to external devices.
- (4) Main switch




5-23 Handpiece (assistant holder)

Vacuum handpiece

Take the vacuum handpiece out of the assistant holder, and suction will start. Since a delay circuit is provided, suction does not stop immediately when the vacuum handpiece is returned to the assistant holder. Suction will continue for approx. 4 seconds.

The suction volume may be controlled by opening or closing the valve.




Saliva ejector handpiece

Take the saliva ejector handpiece out of the assistant holder, and suction will start.

Since a delay circuit is provided, suction does not stop immediately when the saliva ejector handpiece is returned to the assistant holder. It will continue for approx. 4 seconds.

The suction volume may be controlled by opening or closing the valve.




5-24 Assistant hose clamp

It is possible to fix the hose to prevent the handpiece hoses from contacting to the floor.

Assistant hose clamp is detachable from the frame, which is suitable for cleaning. [Reference] Assistant hose clamp [page 242]




Touch panel



switch

Assistant control panel

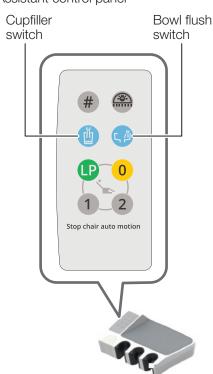

5–25 Filling a Cup

The following two methods can be selected to fill a cup:

- Auto-cupfiller with sensor control: Place a cup on the base, and it will be filled with water to the specified level. (Cup, water level detection)
- Manual cupfiller: Press the cupfiller switch to fill with water for a specified time.

	Cup-filling method
Auto-cupfiller with sensor control (Cup, water level detection)	When a cup is placed on the cupfiller base, a sensor detects the cup, and fills it with the specified quantity of water. To interrupt filling, press the cupfiller switch on the touch panel or assistant control panel. When a cup with some water remaining in it is placed on the cupfiller base, it will be filled with the correct reduced quantity of water. * Even when a fully-filled cup is placed on the base, a small quantity water will be supplied to detect the water level. [Ref] Setting the cupfiller water level [page 213]
Manual cupfiller	When the cupfiller switch (1) on the touch panel or assistant control panel is pressed, water is supplied for the specified time. To interrupt filling, press the cupfiller switch (1) again.

If "cuspidor bowl flush" is set to "continuous flush," water is supplied from the bowl flush nozzle to flush the cuspidor bowl while the cup is filled.

To interrupt the flush, press the bowl flush switch [4] (4) on the touch panel or assistant control panel.

If any droplet or dirt is attached on the surface of cupfiller sensor, the cupfiller may not work properly. In that case, wipe off the droplet or dirt after switching the sensor into disable mode.

Sensor disable mode (Cupfiller base maintenance mode)

The sensor disable mode can be activated by holding down the cupfiller switch on the touch panel or assistant control panel for 2 seconds or more. In the sensor disable mode, continuous bleeps are emitted, and sensor control is disabled for the auto-cupfiller. The LED indicator on the cuspidor unit displays pink.

To terminate the sensor disable mode, press the cupfiller switch <u>i</u> again. The LED indicator returns to its original color.

LED indicator

5-26 LED indicator

Color of the LED indicators show the status of the unit/chair.



All the functions are correctly provided.

[ON, Orange]

The system is in either of the states described below:

- The chair lock function is activated.
- The handpiece lock function is activated.

[Ref] Chair lock function [pages 111 to 114] Handpiece lock function [page 115]

[Flickering Orange]

Water level in the water bottle is low.

[ON, Pink]

The system is in either of the states described below:

- Sensor control for the auto-cupfiller is in the sensor disable mode.
- Operation mode of the dental light is in the switch mode.
- The cupfiller water level is now being set.

[Ref] Sensor disable mode [page 153]

Operation mode of the dental light [page 98] Setting the cupfiller water level [page 213]

Since the color of the LED indicator gives an indication of the status of the chair/handpiece lock or mode transition, always check that the LED indicator is functioning correctly before starting daily work.







Pink




5-27 Water bottle


Refill water when the water bottle level becomes low.


Replacing the water bottle

[How to remove the water bottle]


(1) Flip the BOTTLE AIR switch downward (OFF).







[How to attach it] Reattach it in the reverse order of (1) to (4).



* When not using the water from the water bottle, flip the WATER toggle switch backward (CITY).

Instrument delivery Holder




5-28 USB port


The USB port accepts a doctor table for a USB-type intraoral camera or other device.

Connecting cable should be necessary inside doctor table as per the specification of the device to be added.

Instrument delivery









Turn on the product's main switch; the dental light comes on and the indicator lights up.

The dental light can be turned on or off using the touchless switch or the dental light switch (as a sistant control panel).

Turning the dental light on or off with the touchless switch.

The touchless switch is activated by a sensor. The sensor detects an object of the same width as the sensor window at a distance of approx. 65 mm or closer. Move a hand across the switch to turn it on, and again to turn it off.

* If the surface of the touchless switch is dirty, it may degrade the sensitivity of the switch. If the surface is dirty, clean it with a soft cloth.

Adjusting illuminance in the treatment mode

The illuminance can be adjusted by turning the illuminance controller.

The illuminance cannot be adjusted when the light is turned on under ON mode.

Switching from the treatment mode to Composite-Safe mode

Hold your hand over the touchless switch within the 65-mm range for the specified time, or press the dental light switch and on the touch panel of the assistant control panel for the specified time to change operation to the Composite-Safe mode.


The illuminance cannot be adjusted when the light is turned on under Composite-Safe mode.

Repeat the above step to switch operation back to the treatment mode.

* When the light is turned off in the Composite-Safe mode and turned on again, it will be in the treatment mode.



Before use, always read the Instructions for each dental light to ensure correct usage.





5–30 900 Dental Light

Turn on the product's main switch; the dental light turns on and the indicator displays in green.

The dental light can be turned on or off using the touchless switch or the dental light switch (as a control panel) or assistant control panel.

Turning the dental light on or off with the touchless switch.

The touchless switch is activated by a sensor. The sensor detects an object at distance of approx. 65 mm or closer from the switch. Move a hand across the switch to turn it on, and again to turn it off.

* If the surface of the touchless switch is dirty, it may degrade the sensitivity of the switch. If the surface is dirty, clean it with a soft cloth.

Adjusting the illuminance in the treatment mode

The illuminance can be adjusted by turning the illuminance controller.

The illuminance cannot be adjusted when the light is turned on under ON mode.

Switching from the treatment mode to Composite-Safe mode

Hold your hand over the touchless switch within the 65-mm range for the specified time, or press the dental light switch assistant control panel for the specified time to switch operation to the Composite-Safe mode; the indicator flickers in green.

The illuminance cannot be adjusted when the light is turned on under Composite-Safe mode.


Repeat the above step to switch operation to the treatment mode; the indicator turns steady green.

Mode	Indicator
Treatment mode	ON, Green
Composite-Safe mode	Flickering Green

* When the light is turned off in the Composite-Safe mode and turned on again, it will be in the treatment mode.



Before use, always read the Instructions for Use supplied with each dental light to ensure correct usage.



5–31 Monitor bracket

The monitor can be swung to a position where you can easily see it. When adjusting the position, hold the monitor while you move it.

When moving the monitor, do not let it touch the wall or other object.




CAUTION

Do not apply an excessive load or shock to the monitor or monitor bracket. To avoid damage or injury, ensure that the monitor satisfies the following specifications:

Size: Up to 340 x 530 mm (L x W) [22-inch or smaller monitor]

Weight: Up to 6.5 kg

* Excluding dimensions of monitor handle and other accessories




5-32 Panoramic viewer

Turn the switch upward to turn on the screen and downward to turn it off.

Turn the luminance controller upward to increase the luminance and downward to lower it.

When it is not being used, turn it off.

The panoramic viewer is designed to supplement X-ray observation and is not for examination or diagnosis.



5-33 Dental viewer

Press the switch to turn the screen on. Press it again to turn the screen off.

When it is not being used, turn it off.

The dental viewer is designed to supplement X-ray observation and not for examination or diagnosis.

5-34 Right/Left handed dentistry conversion

Please confirm before converting to right or left handed position.

Bring the chair to the lower limit position and backrest upright position.

Turn off the main switch for safety.

Confirm that there are no obstacles around this product.



CAUTION

Take care so the unit does not make contact with other people or obstacles during the conversion. It may cause damage to the unit or physical injury.

Right/Left handed dentistry conversion

Base mount

Example: Change from right handed position to left handed position for standard package.

1. Pull up the lock lever C on the swing arm bracket to unlock.

The lock lever C may be difficult to pull up. In that case, pull up the lock lever C while adjusting the position of the light pole.



2. Lift the toe board of the seat cushion and swing the light pole to the other side as shown on the left figure.

When the light pole reaches the correct position as shown on the left figure, the lock lever C on the swing bracket will lock automatically.



3. After moving the light pole, adjust the position of the balance arm to position as shown on the left figure.



5 Operation




4. Swing the assistant holder behind the backrest as shown on the left figure.



CAUTION

Take care not to pinch the vacuum hose and saliva ejector hose between the assistant arm and the cuspidor swing arm during the conversion.



5. Pull forward the lock lever B on the bottom of the cuspidor unit until the red mark is seen, then turn the lock lever B so the hollow comes to the upside position.



Lock



The lock lever B may be difficult to pull. In that case, pull forward the lock lever B while adjusting the position of the cuspidor body.




6. Swing the doctor table to the cuspidor side as shown on the left figure.




CAUTION

Take care so the doctor table does not hit the cuspidor during the conversion.



7. Remove the swing bracket cover by pulling in the direction of the arrow. Pull up the lock lever A and turn it until the lever is locked in place.

The lock lever A may be difficult to pull up. In that case, pull up the lock lever A while adjusting the position of the swing bracket.





8. Swing the cuspidor unit behind the chair as shown on the left figure.



CAUTION


Take care so the cuspidor unit does not hit the doctor table during the conversion.



9. Switch the position of the assistant holder to the other side. At that time, the vacuum hose and saliva ejector hose will twist. Pick them up from the assistant holder to remove the twist.



10. Swing the cuspidor unit and the assistant holder as shown on the left figure. When the cuspidor unit reaches the correct position as shown on the left figure, the lock lever A on the swing bracket will lock automatically. Refer to the step 11 for the lock position of the cuspidor unit.



11. Turn the lock lever B so the hollow comes to the downside position. The lock lever B may not return to lock position. In that case, adjust the position of the cuspidor body until the lock lever B is back in lock position.



ock Unlock

5 Operation



12. Attach the swing bracket cover to the swing bracket.

The swing bracket cover is the same for left and right. Turn the cover upside down and attach it.

After the conversion, be sure to confirm that the safety functions are working properly. Please refer to the next page.

Confirm the safety functions

For safe use of this product, please confirm the safety functions as follows after every conversion.

In the following conditions, make sure that the touch panel shows a chair lock screen, and that the chair motions do not function.

Refer to page 112 for chair motion stop function.




(1) When excess pressure (upward or downward) is applied to the doctor table.



(2) When the doctor table is turned to the back side of the backrest.

5 Operation



Swing mount

Example: Change from left handed position to right handed position for standard package.

1. Move the doctor table as shown on the left figure.



2. Pull up the lock lever C on the swing arm bracket to unlock.

The lock lever C may be difficult to pull up. In that case, pull up the lock lever C while adjusting the position of the light pole.



3. Lift the toe board of the seat cushion and swing the light pole to the other side as shown on the left figure.

When the light pole reaches the correct position as shown on the left figure, the lock lever C on the swing bracket will lock automatically.





4. After moving the light pole, adjust the position of the balance arm to position as shown on the left figure.



5. Swing the doctor table to the cuspidor side as shown on the left figure.




Take care so the doctor table does not hit the cuspidor during the conversion.



6. Swing the assistant holder behind the backrest as shown on the left figure.



Take care not to pinch the vacuum hose and saliva ejector hose between the assistant arm and the cuspidor swing arm during the conversion.



Lock

Unlock

7. Pull forward the lock lever B on the bottom of the cuspidor unit until the red mark is seen, then turn the lock lever B so the hollow comes to the upside position.

The lock lever B may be difficult to pull. In that case, pull forward the lock lever B while adjusting the position of the cuspidor body.

5 Operation




Swing bracket cover

8. Remove the swing bracket cover by pulling in the direction of the arrow. Pull up the lock lever A and turn it until the lever is locked in place.

The lock lever A may be difficult to pull up. In that case, pull up the lock lever A while adjusting the position of the swing bracket.





9. Swing the cuspidor unit behind the chair as shown on the left figure.



CAUTION

Take care so the cuspidor unit does not hit the doctor table during the conversion.




10. Switch the position of the assistant holder to the other side. At that time, the vacuum hose and saliva ejector hose will twist. Pick them up from the assistant holder to remove the twist.

5 Operation



11. Swing the cuspidor unit and the assistant holder as shown on the left figure. When the cuspidor unit reaches the correct position as shown on the left figure, the lock lever A on the swing bracket will lock automatically. Refer to the step 12 for the lock position of the cuspidor unit.



Lock

Unlock

12. Turn the lock lever B so the hollow comes to the downside position. The lock lever B may not return to lock position. In that case, adjust the position of the cuspidor body until the lock lever B is back in lock position.



13. Attach the swing bracket cover to the swing bracket.

The swing bracket cover is the same for left and right. Turn the cover upside down and attach it.

Manual control switches





Preset switches



Automatic return switch


6–1 Setting for automatic operation

6–1–1 Setting the treatment and entry/exit positions

- 1. Move the chair to the treatment position or entry/exit position using the manual control switch as required.
- 2. Press and hold the preset switch 1 or 2 (treatment position) or automatic return switch 0 (entry/exit position) for approx. 5 seconds. A beep sounds, and the chair is set to the position.
- 3. Move the chair away from the set position, and press the preset switch to check the chair moves to the set position.

6–1–2 Setting the mouth rinsing position

- 1. Move the chair to the preset mouth rinsing position using the manual control switch.
- 2. Press and hold the last position switch **p** for approx. 5 seconds. A beep sounds, and the chair is set to the position.
- 3. Move the chair away from the set position, and press the last position switch **P** to check the chair moves to the set position.



Manual control switches




Last position switch

Home screen



6–2 Function switch

Press the function switch on the Home screen to display the Function setting screen.




Select an item to display the corresponding setting screen.

Press the switch to cancel operation and return from the current screen to the Home screen.


Press the \supset switch to cancel operation and return from the current screen to the previous screen.

Press the V switch to proceed to the next page.



Press the \wedge switch to return to the previous page.

Press the \vee switch to proceed to the 3rd page.



Press the \wedge switch to return to the 2nd page.

6-2-1 Setting items with the function switch

Setting items appearing on the touch panel		
Flushing, Washing the vacuum line		
Flushing	page 171	
Washing the vacuum line	page 191	
Handpiece		
Drive air pressure	page 208	
Spray mode	page 209	
Handpiece light activation	page 210	
Micromotor light brightness	page 211	
Cup, bowl		
Cupfiller water level	page 213	
Interlock of cup-filling, bowl flush	page 215	
Bowl flush time	page 216	
Language	page 217	
Timer and control panel		
Timer alarm sound	page 218	
Key touch volume	page 219	
Sleep mode time	page 220	
Emergency cancellation chair lock	page 221	
Program version	page 222	
Service mode	*	

^{*} The service mode is designed exclusively for service engineers to carry out maintenance on this product.



6–2–2 Selecting the flushing method and carrying out flushing

Cuspidor Unit type

To flush the water circuit of the handpiece alone

1. Press the function switch .


The Function setting screen appears.




2. Press the 'Flushing, Washing the vacuum line' switch.

If the washing function for vacuum line is not equipped, 'Flushing' appears on the screen instead.

Procedures shown below are not applicable.




3. Press the 'Flushing' switch.



4. Check "Handpieces 00:40" is selected and press OK switch.


To change time setting [Reference] Timer setting of flushing (handpiece) [pages 181,182]



* When using the timer, the screen shown in the figure on the left is displayed.

Press x to cancel flushing.

Press OK to start flushing.




5. Pick up the handpiece you want to flush, and set it in the cuspidor bowl.


[Reference] Preparing handpieces/syringe for flushing [page 190] Always flush the handpiece with the main body of the ultrasonic scaler attached. Flushing without it may cause a malfunction.


The number of the handpiece you have picked up appears. (Handpieces are numbered 1, 2, 3 and 4 from front left.)

The screen does not return to the Home screen even when the \bigcirc switch is pressed.



Remaining time (e.g. 30 sec.)





6. Step on the pedal of the foot controller.

When the pedal is released, the handpiece continuously discharges water for 40 seconds.

The screen does not return to the previous screen even when the \supset switch is pressed.

- * To suspend flushing, press the switch on the touch panel, the membrane switch, or either switch on the assistant panel, or step on the foot controller pedal.
- * To resume flushing, press the switch.
- * To terminate flushing prematurely after pressing ______, press ______, press ______, membrane switch / assistant operation panel switch, or step on the foot controller.
- * To terminate flushing prematurely without pressing _____, press the membrane switch/assistant operation panel switch, or step on the foot controller.
- 7. Once flushing is completed, return the handpiece to the instrument holder. When the handpiece is returned, the home screen appears.
- * Water is not automatically discharged from the syringe. Press the W lever/button for 40 seconds to discharge.

Flushing the water circuits of the handpiece and the cupfiller

This mode is to fill the unit with chemical solution of the water bottle for water bottle specification.

- * Place a cup on the cupfiller base
- 1. Press the function switch .

The Function setting screen appears.







2. Press the 'Flushing, Washing the vacuum line' switch.

If the washing function for vacuum line is not equipped, 'Flushing' appears on the screen instead.

Procedures shown below are not applicable.




3. Press the 'Flushing' switch.



4. Check "Handpieces and Cupfiller 00:30" is selected and press ok switch.


switch.

To change time setting [Reference] Timer setting of flushing (handpiece + cupfiller) [pages 183,184]



If the water bottle specification is not installed, the screen on the left will be displayed.


The following procedure does not apply.



* When using the timer, the screen shown in the figure on the left is displayed.

Press x to cancel flushing.

Press OK to start flushing.



5. Pick up the handpiece you want to flush, and set it in the cuspidor bowl.

[Reference] Preparing handpieces/syringe for flushing [page 190] Always flush the handpiece with the main body of the ultrasonic scaler attached. Flushing without it may cause a malfunction.

The number of the handpiece you picked up appears. (Handpieces are numbered 1, 2, 3 and 4 from front left.)

The screen does not return to the Home screen even when the $\widehat{\Box}$ switch is pressed.

Before starting flushing, always place a cup on the cupfiller base. Without a cup, water will splash onto the wall or chair.



Status of handpiece flushing


Remaining time (e.g. 10 sec.)

6. Step on the pedal of the foot controller.

When the pedal is released, the handpieces continuously discharge water for 20 seconds. Then the cupfiller nozzle discharge water for 10 seconds.

The screen does not return to the previous screen even when the switch \supset is pressed.

- * To suspend flushing, press the switch on the touch panel, the membrane switch, or either switch on the assistant panel, or step on the foot controller pedal.
- * To resume flushing, press
- * To terminate flushing prematurely after pressing ______, press ______, membrane switch/assistant operation panel switch, or step on the foot controller.
- * To terminate flushing prematurely without pressing ______, press the membrane switch/assistant operation panel switch, or step on the foot controller.



Cupfiller status



7. Once flushing is completed, return the handpiece to the instrument holder. When the handpiece is returned, the home screen appears.

* Water is not automatically discharged from the syringe. Press the W lever/button for 40 seconds to discharge.



Flushing the water circuits of the handpiece and the cupfiller/cuspidor bowl

- * Place a cup on the cupfiller base
- 1. Press the function switch .


The Function setting screen appears.




2. Press the 'Flushing, Washing the vacuum line' switch.

If the washing function for vacuum line is not equipped, 'Flushing' appears on the screen instead.

Procedures shown below are not applicable.




3. Press the 'Flushing' switch.



4. Check "HP, Cupfiller and Bowl flush nozzle 05:20" is selected and press ok switch.

To change timer setting

[Reference] Timer setting of flushing (handpiece + cupfiller + cuspidor bowl) [pages 185,186]



- * When using the timer, the screen shown in the figure on the left is displayed.
- Press (x) to cancel flushing.

Press ok to start flushing.



5. Pick up the handpiece you want to flush, and set it in the cuspidor bowl.

[Reference] Preparing handpieces/syringe for flushing [page 190]
Always flush the handpiece with the main body of the ultrasonic scaler attached.
Flushing without it may cause a malfunction.

The number of the handpiece you picked up appears. (Handpieces are numbered 1, 2, 3 and 4 from front left.)

The screen does not return to the Home screen even when the $\widehat{\Box}$ switch is pressed.

Before starting flushing, always place a cup on the cupfiller base. Without a cup, water will splash onto the wall or chair.

Flushing Flushing in progress Output Output

Remaining time (e.g. 4 min.)

6. Step on the pedal of the foot controller.

When the pedal is released, the handpieces continuously discharge water for 2 minutes 40 seconds. Then the cupfiller nozzle and bowl flush nozzle discharge water for 2 minutes 40 seconds.

The screen does not return to the previous screen even when the switch \supset is pressed.

- * To suspend flushing, press the switch on the touch panel, the membrane switch, or either switch on the assistant panel, or step on the foot controller pedal.
- Flushing 全面点点 05:20 中 5

 Flushing in pause

 02:40
 以及 01:30

Cupfiller and bowl flush status

- * To resume flushing, press .
- * To terminate flushing prematurely after pressing ______, press ______, press ______, membrane switch / assistant operation panel switch, or step on the foot controller.
- * To terminate flushing prematurely without pressing ______, press the membrane switch/assistant operation panel switch, or step on the foot controller.



7. Once flushing is completed, return the handpiece to the instrument holder. When the handpiece is returned, the home screen appears.

* Water is not automatically discharged from the syringe. Press the W lever/button for 40 seconds to discharge.



To flush the water circuit of the handpiece alone (Short mode)

1. Press the function switch .

The Function setting screen appears.




Function setting

Flushing

Handpiece

Language


2. Press the 'Flushing' switch.



3. Check "Handpieces Short mode 00:40" is selected and press OK switch.

To change timer setting


[Reference] Timer setting of flushing (Vac Pac unit type / without cuspidor bowl type) [pages 187,188]



* When using the timer, the screen shown in the figure on the left is displayed.

Press x to cancel flushing.

Press OK to start flushing.




4. Pick up the handpiece you want to flush, and set it in the container, such as a bucket.


[Reference] Preparing handpieces/syringe for flushing [page 190] Always flush the handpiece with the main body of the ultrasonic scaler attached. Flushing without it may cause a malfunction.


The number of the handpiece you have picked up appears. (Handpieces are numbered 1, 2, 3 and 4 from front left.)

The screen does not return to the Home screen even when the $\widehat{\ }$ switch is pressed.



Remaining time (e.g. 30 sec.)





5. Step on the pedal of the foot controller.

When the pedal is released, the handpiece continuously discharges water for 40 seconds.

The screen does not return to the previous screen even when the \supset switch is pressed.

- * To suspend flushing, press the switch on the touch panel, the membrane switch, or either switch on the assistant panel, or step on the foot controller pedal.
- * To resume flushing, press the switch.
- * To terminate flushing prematurely after pressing , press / membrane switch / assistant operation panel switch, or step on the foot controller.
- * To terminate flushing prematurely without pressing ______, press the membrane switch/assistant operation panel switch, or step on the foot controller.
- 6. Once flushing is completed, return the handpiece to the instrument holder. When the handpiece is returned, the home screen appears.


^{*} Water is not automatically discharged from the syringe. Press the W lever/button for 40 seconds to discharge.




To flush the handpiece + unit water circuit (Long mode)

1. Press the function switch .

The Function setting screen appears.




2. Press the 'Flushing' switch.



3. Check "Handpieces Long mode 02:40" is selected and press ok switch.

To change timer setting


[Reference] Timer setting of flushing (Vac Pac unit type / without cuspidor bowl type) [pages 187,188]



* When using the timer, the screen shown in the figure on the left is displayed.

Press x to cancel flushing.

Press **OK** to start flushing.



4. Pick up the handpiece you want to flush, and set it in the container, such as a bucket.

[Reference] Preparing handpieces/syringe for flushing [page 190] Always flush the handpiece with the main body of the ultrasonic scaler attached. Flushing without it may cause a malfunction.

The number of the handpiece you have picked up appears. (Handpieces are numbered 1, 2, 3 and 4 from front left.)

The screen does not return to the Home screen even when the $\widehat{\Box}$ switch is pressed.

5

02:40


):30


Remaining time (e.g. 30 sec.)

Flushing

Long mode

Flushing in progress





5. Step on the pedal of the foot controller.

When the pedal is released, the handpiece continuously discharges water for 2 minutes 40 seconds.

The screen does not return to the previous screen even when the \supset switch is pressed.

- * To suspend flushing, press the switch on the touch panel, the membrane switch, or either switch on the assistant panel, or step on the foot controller pedal.
- * To resume flushing, press the switch.
- * To terminate flushing prematurely after pressing ______, press ______, press ______, membrane switch / assistant operation panel switch, or step on the foot controller.
- * To terminate flushing prematurely without pressing ______, press the membrane switch/assistant operation panel switch, or step on the foot controller.
- 6. Once flushing is completed, return the handpiece to the instrument holder. When the handpiece is returned, the home screen appears.
- * Water is not automatically discharged from the syringe. Press the W lever/button for 40 seconds to discharge.



Timer setting of flushing (handpiece)


1. Press the function switch . The Function setting screen appears.




2. Press the 'Flushing, Washing the vacuum line' switch.

If the washing function for vacuum line is not equipped, 'Flushing' appears on the screen instead.

Procedures shown below are not applicable.



- 3. Press the 'Flushing' switch.
 - * To display the explanation of flushing and washing the vacuum line, press the ? switch (refer to page 192).



4. Press the flushing mode item to change the settings.

Press Handpieces.

The color of the mode frame changes and it becomes a selection display.

5. Press the timer setting switch for flushing.

The screen for changing a flushing time appears.



6. Change the timer setting of the handpiece mode

(example) change to 2 min 30 sec

Pressing the _____/ ____ switches to increase or decrease the time in increments of 1 minute for minutes and 10 seconds for seconds.


: Increase set time
: Decrease set time

Set time range 00:40 to 02:40

The factory default setting is 40 seconds.



7. Press Store Switch to save the setting The flushing screen in 4. appears.





Timer setting of flushing (handpiece + cupfiller)


1. Press the function switch . The Function setting screen appears.




2. Press the 'Flushing, Washing the vacuum line' switch.

If the washing function for vacuum line is not equipped, 'Flushing' appears on the screen instead.

Procedures shown below are not applicable.



- 3. Press the 'Flushing' switch.
 - * To display the explanation of flushing and washing the vacuum line, press the ? switch (refer to page 192).



4. Press the flushing mode item to change the settings.

Press Handpieces and Cupfiller.

The color of the mode frame changes and it becomes a selection display.

5. Press the timer setting switch for flushing.

The screen for changing a flushing time appears.



6. Change the timer setting of the handpiece mode


(example) change to 30 sec

Press the _____/___ switches to increase or decrease the time in increments of 1 minute for minutes and 10 seconds for seconds.

: Increase set time
: Decrease set time

Set time range 00:20 to 05:00

The factory default setting is 20 seconds.



7. Press Cupfiller switch

The color of the mode frame changes and it becomes a selection display.



8. Change the timer setting of the cupfiller mode.

(example) change to 20 sec


Press the _____/___ switches to increase or decrease the time in increments of 1 minute for minutes and 10 seconds for seconds.

: Increase set time
: Decrease set time

Set time range 00:10 to 05:00

The factory default setting is 10 seconds.





9. Press Store Switch to save the setting

The flushing screen in 4. appears.



Timer setting of flushing (handpiece + cupfiller + cuspidor bowl)

1. Press the function switch . The Function setting screen appears.




2. Press the 'Flushing, Washing the vacuum line' switch.

If the washing function for vacuum line is not equipped, 'Flushing' appears on the screen instead.

Procedures shown below are not applicable.



- 3. Press the 'Flushing' switch.
 - * To display the explanation of flushing and washing the vacuum line, press the ? switch (refer to page 192).



- 4. Press the flushing mode item to change the settings.
 - Press HP, Cupfiller and Bowl flush nozzle.

The color of the mode frame changes and it becomes a selection display.

5. Press the timer setting switch for flushing.

The screen for changing a flushing time appears.



6. Change the timer setting of the handpiece mode

(example) change to 3 min

Press the \(\strict{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sq}}}}}}}}}}} \signtimes\sqnt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sq}}}}}}}}}}} \signtimes\sintitex{\sintitex{\sqrt{\sq}}}}}}}}} \end{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sq}}}}}}}}} \end{\sqrt{\sqnt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sq}}}}}}}}} \end{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sqrt{\sq}}}}}}}}} \end{\sqrt{\sqrt{\sq}} increments of 1 minute for minutes and 10 seconds for seconds.

: Increase set time : Decrease set time


Set time range 02:40 to 05:00

The factory default setting is 2 minutes 40 seconds.



7.Press Cupfillier, Cuspidor bowl washing switch [4].

The color of the mode frame changes and it becomes a selection display.



8. Change the timer setting of the cupfiller, cuspidor bowl washing mode. (example) change to 3 min

Press the \(\sim \) switches to increase or decrease the time in increments of 1 minute for minutes and 10 seconds for seconds.


: Increase set time : Decrease set time

Set time range 02:40 to 05:00

The factory default setting is 2 minutes 40 seconds.








◆ 9. Press Store Switch to save the setting The flushing screen in 4. appears.




Timer setting of flushing (Vac Pac unit type / without cuspidor bowl type)

1. Press the function switch . The Function setting screen appears.



2. Press the 'Flushing' switch.



- Press the flashing mode item to change the settings.
 (example) press Handpieces Short mode
 The color of the mode frame changes and it becomes a selection display.
 - * To display the explanation of flushing (Vac Pac unit type / without cuspidor bowl type), press the ? switch (refer to page 189).
- 4. Press the timer setting switch for flushing. The screen for changing a flushing time appears.



5. Change the timer setting

(example) change to 50 sec

Press the switches to increase or decrease the time in increments of 1 minute for minutes and 10 seconds for seconds.

: Increase set time
: Decrease set time


Set time range

Short mode 00:40 to 02:40 Long mode 02:40 to 05:00


The factory default setting is 40 seconds.



6. Press Store Switch to save the setting The flushing screen in 3. appears.




Explanation of flushing (Vac Pac unit type / without cuspidor bowl type)



1. Press ✓ switch

Proceed to the screen in 2.


The explanation of "Handpieces long mode" of flushing appears.



2. Press ∧ switch

Return to the screen in 1.

The explanation of "Handpieces short mode" of flushing appears.




3. Press > switch

Return to the screen in 3. in page 187.

Preparing handpieces/syringe for flushing

Set the right side of the detaching position in the cuspidor bowl.

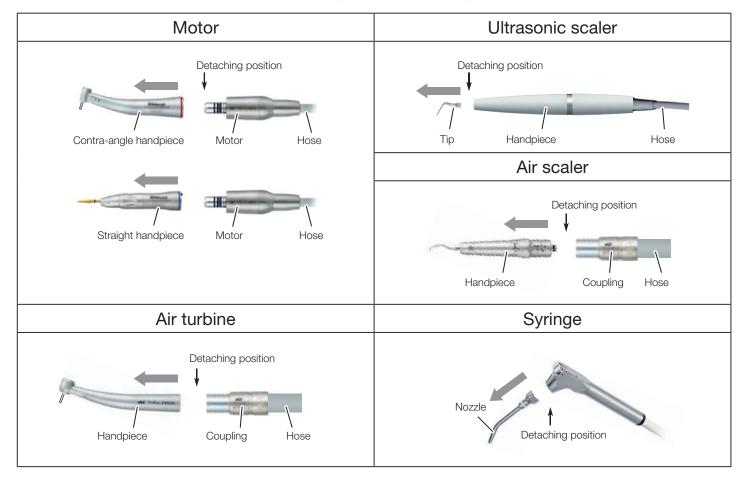

After flushing, wipe the handpiece with a soft cloth to remove excess moisture.

When picking up the handpiece after flushing, remaining air may be discharged. This is normal.

6–2–3 Selecting the vacuum line washing method and conducting washing

Washing the vacuum line only

The following three options are available: Rinse the vacuum line+wash the vacuum line with cleaner (refer to page 193), Rinse the vacuum line (refer to page 196), and Wash the vacuum line with cleaner (refer to page 198).

Use the one of the following chemical solutions specified by us.


Chemical solution: Orotol plus by Dürr

GREEN&CLEAN M2 by METASYS GREEN&CLEAN CL N by METASYS




1. Press the function switch .


The Function setting screen appears.



2. Press the 'Flushing, Washing the vacuum line' switch.




- 3. Press the 'Washing the vacuum line' switch.
- * To display the explanation of flushing and washing the vacuum line, press the ? switch (refer to page 192).



* If you select 'Washing the vacuum line', the amount of remaining cleaner will be checked. If the amount of cleaner is sufficient, the screen shown in the left figure appears.


The name of the set chemical solution is displayed. To change the chemical solution, contact your local authorized Belmont dealer.

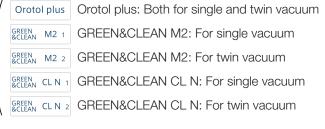


If the amount of cleaner is insufficient, the screen shown in the left figure appears. Refill the cleaner.

[Reference] How to refill the cleaner [page 207]

After refilling the cleaner, press the switch to display the 'Washing the vacuum line' screen.






Explanation of flushing and washing the vacuum line

Press the
 ✓ switch.

The display moves to screen 2.


The explanation of "HP, Cupfiller and Bowl flush nozzle" of flushing appears.



2. Press the V switch.

The display moves to screen 3.


The screen provides an explanation about washing the vacuum line; "Rinse and wash the vacuum line with cleaner", and "Rinsing".



3. Press the V switch.

The display moves to screen 4.


The screen provides an explanation about washing the vacuum line; "Washing with cleaner" and "Flushing and washing the vacuum line".



4. Press the ∧ switch.

The display returns to screen 3.


The screen provides an explanation about washing the vacuum line; "Rinse and wash the vacuum line with cleaner", and "Rinsing".



Press the ∧ switch.


The display returns to screen 2.

The explanation of "HP, Cupfiller and Bowl flush nozzle" of flushing appears.



6. Press the switch.


The display returns to screen 3 shown on page 191.



Rinsing the vacuum line+washing the vacuum line with cleaner

1. Press the 'Rinse the vacuum line+wash the vacuum line with cleaner' switch.

The name of the set chemical solution is displayed. To change the chemical solution, contact your local authorized Belmont dealer.

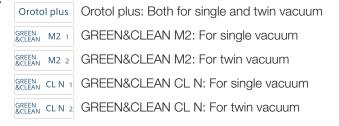



* If the amount of cleaner is insufficient, the screen shown in the left figure appears. Refill the cleaner.


[Reference] How to refill the cleaner [page 207]

- 2. Start rinsing the vacuum line+washing the vacuum line with cleaner.
- ① Open the maintenance panel cover (top) of the cuspidor unit. Pick up the vacuum and saliva ejector handpieces from the assistant holder and insert them into the connector.

[Reference] Procedure for washing with cleaner [page 206] (At this time, the suction is not activated.)



* Before pressing the switch, make sure to insert the vacuum and saliva ejector handpieces into the connector.



* To stop washing the vacuum line in progress, press the 💢 👤 switch.

The displayed time varies depending on the chemical solution.






ejector from the connector.

* If the _____ switch is pressed during washing, the screen shown in the left figure appears.

If the handpiece is removed from the connector while the screen on the left is displayed, the cleaner will be left inside the handpiece and handpiece hose. Leaving the cleaner standing may cause a bacterial growth.




Press the OK switch.



* After the suction starts, return the vacuum and saliva ejector handpieces to the assistant holder.

When the vacuum and saliva ejector handpieces are returned to the assistant holder, the screen returns to the home screen.



3. When you have finished rinsing the vacuum line+washing the vacuum line with cleaner, press the ok switch.



* After the suction starts, return the vacuum and saliva ejector handpieces to the assistant holder.


When the vacuum and saliva ejector handpieces are returned to the assistant holder, the screen returns to the home screen.

After the suction starts, remove the vacuum and saliva ejector handpieces from the connector.

Dripping of the cleaner can be prevented.

If the cleaner drips from the connector, wipe it off immediately.

Places where the cleaner adheres may become discolored.



e.g.

E44: No water in the bottle

5. Press the OK switch.

given.



* After the suction starts, return the vacuum and saliva ejector handpieces to the assistant holder.

When the vacuum and saliva ejector handpieces are returned to the assistant holder, the screen returns to the home screen.


4. In the event of an error state, take appropriate measures.


system will be reset and the error screen will appear.

"Message on the touch panel and measures to be taken"

In the event of an error state before/upon/during washing with cleaner/rinsing, the

Refer to pages 260 to 262 and take measures in accordance with the remedies






Rinsing the vacuum line

1. Press the 'Rinse the vacuum line' switch.

The name of the set chemical solution is displayed. To change the chemical solution, contact your local authorized Belmont dealer.

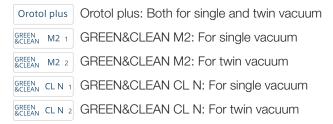

2. Start rinsing the vacuum line.

① Open the maintenance panel cover (top) of the cuspidor unit. Pick up the vacuum and saliva ejector handpieces from the assistant holder and insert them into the connector.

[Reference] Procedure for washing with cleaner [page 206]

- 2 Press the switch.
- * Before pressing the switch, make sure to insert the vacuum and saliva ejector handpieces into the connector.

The screen does not return to the home screen even when the
switch is pressed.



Rinse the vacuum line


Remove the chip/nozzle of the handpieces for vacuum/saliva ejector and insert the handpieces for vacuum/saliva ejector to each connector.

*1 Cover the connector when handpiece for vacuum/saliva is not inserted.

Flushing completes first, then washing

vacuum line follows.

* To stop washing the vacuum line in progress, press the X switch.



* If the _____ switch is pressed during washing, the screen shown in the left figure appears.



Press the OK switch.

* After the suction starts, return the vacuum and saliva ejector handpieces to the assistant holder.

When the vacuum and saliva ejector handpieces are returned to the assistant holder, the screen returns to the home screen.



3. After rinsing of the vacuum line is completed, press the OK switch.



* After the suction starts, return the vacuum and saliva ejector handpieces to the assistant holder.

When the vacuum and saliva ejector handpieces are returned to the assistant holder, the screen returns to the home screen.

After the suction starts, remove the vacuum and saliva ejector handpieces from the connector.

Dripping of the cleaner can be prevented.

If the cleaner drips from the connector, wipe it off immediately.

Places where the cleaner adheres may become discolored.




4. In the event of an error state, take appropriate measures.

In the event of an error state before/upon/during washing with cleaner/rinsing, the system will be reset and the error screen will appear.

"Message on the touch panel and measures to be taken"

Refer to pages 260 to 262 and take measures in accordance with the remedies given.

E44: No water in the bottle




5. Press the OK switch.



* After the suction starts, return the vacuum and saliva ejector handpieces to the assistant holder.


When the vacuum and saliva ejector handpieces are returned to the assistant holder, the screen returns to the home screen.




Washing the vacuum line with cleaner

1. Press the 'Wash the vacuum line with cleaner' switch.

The name of the set chemical solution is displayed. To change the chemical solution, contact your local authorized Belmont dealer.

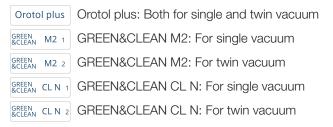



* If the amount of cleaner is insufficient, the screen shown in the left figure appears. Refill the cleaner.

[Reference] How to refill the cleaner [page 207]

2. Start washing the vacuum line with cleaner.


① Open the maintenance panel cover (top) of the cuspidor unit. Pick up the vacuum and saliva ejector handpieces from the assistant holder and insert them into the connector.

[Reference] Procedure for washing with cleaner [page 206] (At this time, the suction is not activated.)



2 Press the switch.


* Before pressing the switch, make sure to insert the vacuum and saliva ejector handpieces into the connector.



The screen does not return to the home screen even when the $\widehat{\square}$ switch is pressed.

* To stop washing the vacuum line in progress, press the Switch.

The displayed time varies depending on the chemical solution.



* If the x switch is pressed during washing, the screen shown in the left figure appears.

If the handpiece is removed from the connector while the screen on the left is displayed, the cleaner will be left inside the handpiece and handpiece hose. Leaving the cleaner standing may cause a bacterial growth.




Press the OK switch.



* After the suction starts, return the vacuum and saliva ejector handpieces to the assistant holder.

When the vacuum and saliva ejector handpieces are returned to the assistant holder, the screen returns to the home screen.



3. When you have finished washing the vacuum line with cleaner, press the $o\kappa$ switch.



* After the suction starts, return the vacuum and saliva ejector handpieces to the assistant holder.


When the vacuum and saliva ejector handpieces are returned to the assistant holder, the screen returns to the home screen.

After the suction starts, remove the vacuum and saliva ejector handpieces from the connector.

Dripping of the cleaner can be prevented.

If the cleaner drips from the connector, wipe it off immediately.

Places where the cleaner adheres may become discolored.




e.g. E44: No water in the bottle 4. In the event of an error state, take appropriate measures.


In the event of an error state before/upon/during washing with cleaner/rinsing, the system will be reset and the error screen will appear.

"Message on the touch panel and measures to be taken"

Refer to pages 260 to 262 and take measures in accordance with the remedies given.



5. Press the OK switch.



* After the suction starts, return the vacuum and saliva ejector handpieces to the assistant holder.

When the vacuum and saliva ejector handpieces are returned to the assistant holder, the screen returns to the home screen.




Flushing and rinsing the vacuum line

1. Press the function switch . The Function setting screen appears.



2. Press the 'Flushing, Washing the vacuum line' switch.



- 3. Press the 'Flushing and washing the vacuum line' switch.
- * To display the explanation of flushing and washing the vacuum line, press the ? switch (refer to page 192).



- 4. Pick up the handpiece you want to flush, and set it in the cuspidor bowl.
 - The number of the handpiece you have picked up appears. (Handpieces are numbered 1, 2, 3 and 4 from front left.)

The screen does not return to the Home screen even when the switch is pressed.

Always flush the handpiece with the main body of the ultrasonic scaler attached. Flushing without it may cause a malfunction.

5. Press the OK switch.



Flushing №点点 05:20 Flushing in progress Status of handpiece flushing Remaining time (e.g. 4 min.)

6. Open the front panel of the cuspidor unit. Pick up the vacuum and saliva ejector handpieces from the assistant holder and insert them into the connector.

Press the switch.

Flushing and rinsing of the vacuum line will start.

* Before pressing the switch, make sure to insert the vacuum and saliva ejector handpieces into the connector.

The screen does not return to the home screen even when the is switch is pressed.

Water flows out of the handpiece for 2 minutes 40 seconds.


Then, water flows out of the cupfiller nozzle and the bowl flush nozzle for 2 minutes 40 seconds.

If the cuspidor bowl is not equipped, rinsing the vacuum line starts 5 minutes after flushing the water circuits of handpieces.

If you need to start rinsing the vacuum line immediately after flushing the water circuits of handpieces, press then press Rinsing the vacuum line starts. [Refer to page 196]

The screen does not return to the previous screen even when the \supset switch is pressed.

- * To suspend flushing, press the switch on the touch panel, the membrane switch, or either switch on the assistant panel, or step on the foot controller pedal.
- * To resume flushing, press the switch.
- * To terminate flushing prematurely after pressing / membrane switch/assistant operation panel switch, or step on the foot controller.
- * To terminate flushing prematurely without pressing membrane switch/assistant operation panel switch, or step on the foot controller.



Cupfiller and bowl flush status


To display the screen in step 6, press the \supset switch.

To display the screen shown in the left figure, press the switch.




When flushing is completed, rinsing of the vacuum line will start.

* To stop rinsing the vacuum line in progress, press the X switch.




* If the x switch is pressed during rinsing, the screen shown in the left figure appears.



Flushing Missing is completed.

Return the handpieces to the handpiece holder.



Press the OK switch.

* After the suction starts, return the vacuum and saliva ejector handpieces to the assistant holder.

When the vacuum and saliva ejector handpieces are returned to the assistant holder, the screen returns to the home screen.



7. After rinsing of the vacuum line is completed, return the handpieces for doctor unit to the instrument holder.

After flushing, if the handpieces are returned to the instrument holder while the vacuum line is being rinsed, the screen shown in the left figure does not appear.

* Water is not automatically discharged from the syringe. Press the W lever/button of the syringe for 40 seconds to discharge.

To display the screen shown in the left figure, press the \supset switch.




Press the OK switch.

The screen in step 6 appears.

To display the screen in step 3, press the \supseteq switch.



8. Press the OK switch.



* After the suction starts, return the vacuum and saliva ejector handpieces to the assistant holder.

When the vacuum and saliva ejector handpieces are returned to the assistant holder, the screen returns to the home screen.


* If the handpieces for doctor unit are returned after the vacuum and saliva ejector handpieces, the home screen appears instead of the screen in step 8.

After the suction starts, remove the vacuum and saliva ejector handpieces from the connector.

Dripping of the cleaner can be prevented.

If the cleaner drips from the connector, wipe it off immediately.

Places where the cleaner adheres may become discolored.



e.g.


E44: No water in the bottle

9. In the event of an error state, take appropriate measures.

In the event of an error state before/upon/during washing with cleaner/rinsing, the system will be reset and the error screen will appear.

"Message on the touch panel and measures to be taken"

Refer to pages 260 to 262 and take measures in accordance with the remedies given.



10. Press the OK switch.




* After the suction starts, return the vacuum and saliva ejector handpieces to the assistant holder.

When the vacuum and saliva ejector handpieces are returned to the assistant holder, the screen returns to the home screen.

(1)









Procedures for washing with cleaner

(1) Open the maintenance panel cover (top) of the cuspidor unit.

- (2) Pick up the vacuum and saliva ejector handpieces from the assistant holder. Remove the vacuum and saliva ejector chips.
- (3) Insert (2) into the connector.

A vacuum connector cap (hereinafter, 'connector cap') should be attached to a connector that is not being used.


Do not remove the connector cap attached to a connector that has no function or a connector that is not being used. Its removal weakens the suction and may hinder suction capacity.

The connector cap may be lost when removed.




- * Do not remove the solid collector while washing. Without the solid collector, the suction does not work.
 - If the solid collector is removed during washing, the washing will not be performed and water may burst forth.
- * Do not remove the handpiece from the connector during washing. An error may

The washing may take longer than the indicated time depending on the vacuum capacity of the machine room.








Cleaner bottle replacement bottle







How to refill the cleaner

- (1) Open the side panel of the cuspidor unit.
 - 1 Loosen the screw.
 - 2 Pull open the side panel toward you.
- (2) Pull down the cleaner bottle panel toward you.
- (3) PPour up to 500 ml of cleaner into the replacement bottle. Place the cap on the bottle and bring the bottle near the cuspidor unit.
- (4) Move the cleaner bottle toward you.

 Place the cleaner and replacement bottles next to each other.
- (5) Remove the cap from the replacement bottle.
- (6) Remove the cover from the cleaner bottle by lifting it up slowly. Attach the cover to (5).
- (7) Move (6) to the place where the used cleaner bottle was originally located.

Besides the bottle in the cuspidor unit, a replacement bottle with a cap is also attached. Store it in a stock room and use it when replacing the cleaner bottle in the cuspidor unit with a new one.

Do not use the chemical solution other than the one already set at the display. The chemical solution set is the one chosen from our specified list. [Reference] Chemical solution specified by us [page 191]

The bottle can contain 500ml of chemical solution. The number of washings depends on the chemical solution.

Place the cap on the remaining bottle. Use the bottle for replacement. Use the cleaner remaining in the replaced bottle when refilling the cleaner the next time.

6–2–4 Displaying the drive air pressure

Display the handpiece drive air pressure.

1. Press the function switch . The Function setting screen appears.



Function setting


Flushing Washing the vacuum line

Spittoon valve cleaning

Handpiece

Language

2. Press 'Handpiece.'



3. Press 'Drive air pressure.'

The Drive air pressure screen appears.



- 4. Pick up the handpiece to measure the pressure from the instrument holder.
- 5. Step on the pedal of the foot controller.

The air pressure is displayed.

During the pedal of foot controller being stepped on, pressing \bigcirc will not bring the mode to home screen; pressing \bigcirc will not bring the mode to the previous screen.

- 6. After checking the pressure, return the handpiece to the instrument holder.
- 7. Press the 🖻 switch to display the Home screen.

6-2-5 Setting the spray mode

Two mode: Spray ON/OFF

Four mode: Air and water ON/OFF

Regardless of two or four modes, an ultrasonic scaler can toggle between ON/ OFF of W(Water) only.

1. Press the function switch .
The Function setting screen appears.




Flushing, Washing the vacuum line

Spittoon valve cleaning


Handpiece

Language

2. Press 'Handpiece.'



- 3. Press 'Spray mode.'
- The Spray Mode setting screen appears.



- 4. Pick up the handpiece you want to set.
- 5. Select 'Two mode' or 'Four mode.'
- 6. Press OK to save the setting. The previous screen appears.
- * To cancel the setting, press \supset without pressing \bigcirc \bigcirc \bigcirc \bigcirc
- 7. Return the handpiece to the instrument holder.
- 8. Press the is switch to display the Home screen.

6-2-6 Setting the light activation timing

Two types of light activation timing can be selected.

'When picking up a handpiece'

Turns on when the handpiece is picked up from the instrument holder and will turn off when returned to the holder.

* For NO PAIN, the light turns off after the afterglow period is completed.

'When stepping on the foot controller'

Turns on while the handpiece is activated and off after the after-glow period (approx. 5 seconds) is completed after the handpiece deactivates.

- * For NO PAIN, the light turns off after the afterglow period is completed.
- * Contact your local authorized Belmont dealer when the setting of afterglow period for NEWTRON/ VARIOS170 should be changed.

 Setting of afterglow period for NO PAIN cannot be changed.
- Patient
 Adult

 Adult

 User

 A User


 Whanual

 Wheater


 Whigh

 Whig

1. Press the function switch . The Function setting screen appears.



2. Press 'Handpiece.'



3. Press 'Handpiece light activation.'

The Handpiece light activation setting screen appears.



- 4. Select 'When picking up a handpiece' or 'When stepping on the foot controller.'
- 5. Press OK to save the setting. The previous screen appears.
- * To cancel the setting, press \supset without pressing \bigcirc κ .
- 6. Press the is switch to display the Home screen.

6–2–7 Setting the micromotor brightness

Handpiece light brightness (illuminance) can be changed.

NLX plus

1. Press the function switch . The Function setting screen appears.



Function setting


Flushing Washing the vacuum line

Spittoon valve cleaning

Handpiece


Language

2. Press 'Handpiece.'



3. Press 'Micromotor light brightness.'

The micromotor light brightness setting screen appears.



- 4. Pick up the handpiece to set.
- 5. Press the _____ switches to adjust the brightness. Adjust the brightness while checking actual brightness.
- * It is not necessary to press OK to save this setting. It is memorized when the brightness (illuminance) is set.
- 6. Press the a switch to return to the Home screen.




MX2/MCX

1. Press the function switch . The Function setting screen appears.



2. Press 'Handpiece.'



3. Press 'Micromotor light brightness.'

The micromotor light brightness setting screen appears.



- 4. Pick up the handpiece you want to set.
- 5. Press the memory switch M1 to select [M1], [M2], [M3], or [M4]. These four switches appear sequentially every time the [M1] switch is pressed.
- 6. Press the _____ switches to adjust the brightness between [0] and [15].

The brightness can be adjusted by [1] increment.

7. Press OK to save the setting.

The previous screen appears.

- * To cancel the setting, press $\stackrel{\frown}{\longrightarrow}$ without pressing $\stackrel{\bigcirc}{\bigcirc}$ or
- 8. Press the in switch to return to the Home screen.



The cupfiller water level setting is set on shipment from the factory but may be adjusted as required.

The cupfiller water level and filling duration when using the cupfiller switch (forced cup-filling) can be adjusted.

Patient
Adult

Adult

User

A User

Whanual

Wheater
OFF

Whigh

Whigh

1. Press the function switch . The Function setting screen appears.

Function setting

Flushing Washing the vacuum line


Spittoon valve cleaning

Handpiece


Language

2. Press the V switch.

The second page of the Function setting screen appears.



3. Press 'Cupfiller, bowl flush.'




4. Press 'Cupfiller water level.'

The Cupfiller water level setting screen appears.



- 5. Place an empty cup on the cupfiller base, and press and hold the <u>u</u> switch to fill the cup to the desired level.
- * Water is supplied while the <u>u</u> switch is pressed and stops when it is released.



- * To memorize the cupfiller water level, press OK . After pressing OK , the previous screen appears.
- * To cancel the setting, press \supset without pressing \bigcirc **o** κ . After pressing \supset , the previous screen appears.

6. Press the figure switch to return to the Home screen.

If the water supplied exceeds the desired water level, set it again from the beginning.

To cancel the setting in the middle, press \bigcirc or \bigcirc .

6–2–9 Setting the cup-filling/bowl flush interlock

The following two modes can be selected:

'Interlock'


Cuspidor bowl flush starts at the same time as cup-filling.

'No interlock'

The cuspidor bowl is not flushed even when cup-filling is started.




1. Press the function switch . The Function setting screen appears.




2. Press the V switch.

The second page of the Function setting screen appears.




3. Press 'Cupfiller, bowl flush.'



4. Press 'Interlock of cup filling, bowl flush.'


The Interlock of cup filling, bowl flush screen appears.



- 5. Select 'Interlock' or 'No interlock.'
- 6. Press OK to save the setting. The previous screen appears.

_


- * To cancel the setting, press \supset without pressing \bigcirc or
- 7. Press the 💼 switch to return to the Home screen.



Duration of the bowl flush can be set.


1. Press the function switch .
The Function setting screen appears.






2. Press the V switch.

The second page of the Function setting screen appears.




3. Press 'Cupfiller, bowl flush.'



4. Press 'Bowl flush time.'

The Bowl Flush Time setting screen appears.



- 5. Press the switches to set the time between [0] and [15] seconds.
- 6. Press OK to save the setting.

The previous screen appears.

- * To cancel the setting, press \supset without pressing $\bigcirc \kappa$.
- 7. Press the in switch to return to the Home screen.

6 Setting/Adjustment

6-2-11 Setting the language


Language displayed on the touch panel can be changed.





2. Press 'Language.'

The Language setting screen appears.



- 3. Press the \(\cdot \) \(\chi \) switches to select your language.
- 4. Press OK to save the setting. The previous screen appears.
- * To cancel the setting, press \supset without pressing $\bigcirc \kappa$.
- 5. Press the switch to return to the Home screen.

6-2-12 Setting the timer alarm tone

Alarm tone emitted when the timer reaches zero can be set.

Five tones are available and can be set to distinguish between different chairs in the same room.




1. Press the function switch .

The Function setting screen appears.




2. Press the ∨ switch.

The second page of the Function setting screen appears.



3. Press 'Timer, control panel.'



4. Press 'Timer alarm selection.'


The Timer Alarm Selection setting screen appears.



- 5. Press the \checkmark switches to select a tone from five types (' $\ifmmode \ensuremath{)}\else$ 1' to ' $\ifmmode \ensuremath{)}\else$ 5').
- 6. Press OK to save the setting.

The previous screen appears.


- * To cancel the setting, press \supseteq without pressing $\bigcirc \kappa$.
- 7. Press the in switch to return to the Home screen.



The tone emitted when a switch is pressed can be set.


1. Press the function switch . The Function setting screen appears.






2. Press the V switch.

The second page of the Function setting screen appears.




3. Press 'Timer, control panel.'



4. Press 'Key touch volume.'

The Key touch volume setting screen appears.



5. Press touch bar graph to set the volume in five levels ('1' to '5').

The witch makes the sound of the tone.

The grant switch mutes the tone.

To mute the tone, press $| \P \rangle$ and the display changes to $| \P \rangle$.

6. Press OK to save the setting.


The previous screen appears.

- * To cancel the setting, press \supset without pressing \bigcirc oK \bigcirc .
- 7. Press the a switch to return to the Home screen.

6-2-14 Setting the sleep mode time


When no switch on the control panel is used for a while, the touch panel screen goes dark and enters the sleep mode. The time before entering sleep mode can be adjusted.

1. Press the function switch . The Function setting screen appears.




2. Press the ∨ switch.

The second page of the Function setting screen appears.




3. Press 'Timer, control panel.'



4. Press 'Sleep mode time.'

The Sleep mode time setting screen appears.



- 5. Press the Switches to select one of three durations ('5 min,' '10 min,' and '15 min').
- 6. Press OK to save the setting. The previous screen appears.
- * To cancel the setting, press $\stackrel{\frown}{\bigcirc}$ without pressing $\stackrel{\frown}{\bigcirc}$ or $\stackrel{\frown}{\bigcirc}$.
- 7. Press the switch to return to the Home screen.
- * To cancel the sleep mode, touch the screen.


6 Setting/Adjustment

6-2-15 Setting emergency cancellation of the chair lock

The chair lock function, when activated, can be temporarily cancelled. Use this temporary cancellation only when the chair lock function must be disabled to resolve a malfunction.




1. Press the function switch . The Function setting screen appears.




2. Press the V switch.

The second page of the Function setting screen appears.



3. Press 'Emergency cancellation of chair lock.'

The Emergency cancellation of chair lock setting screen appears.



- 4. Press the Switches to cancel the chair lock. [Reference] Chair lock function [pages 112 to 114]
- 5. Press the OK switch to save the setting. The previous screen appears.
- * To cancel the setting, press $\stackrel{\frown}{\longrightarrow}$ without pressing $\stackrel{\frown}{\bigcirc}$ or $\stackrel{\frown}{\bigcirc}$.
- 6. Press the 🖻 switch to return to the Home screen.
- * When the main switch is turned off, emergency cancellation of the chair lock will be disabled, and the chair lock function will be reactivated.

Patient

6-2-16 Displaying the program version

The program version of each circuit board installed inside the unit can be checked.



∭ High

1. Press the function switch .


The Function setting screen appears.



[∭] Heater ☐ **OFF**


2. Press the V switch.

The second page of the Function setting screen appears.



3. Press 'Program version'.

The screen to check the program version appears.



4. Check the program version.

(example) LCD Main ver is TB220514

ID : TB2205 Major : 1 Full : 1.4

Press the V switch to proceed to the 2nd page.



Press the \wedge switch to return to the 1st page.

5. Press the a switch to display the home screen.




6–3 Adjusting the quantity of water/air supplied from the doctor unit

Adjusting the quantity of water /air supplied to the syringe spray


The quantity of water and air supplied from the doctor unit can be adjusted with the knobs (1).

Blue cap (W side): Quantity of water supplied Yellow cap (A side): Quantity of air supplied



Adjusting the quantity of water supplied to the handpiece spray

The quantity of water supplied to the handpiece spray from the doctor unit can be adjusted with the knobs (2) (with blue caps).



Holder



Place holder



Syringe 1 2 3 4 1 2 3 4 Syringe All the knobs decrease the flow rate when turned clockwise and increase it when turned counterclockwise.

Do not close the adjusting knob too tightly. It is used to increase or decrease flow rate and is not a stop valve. Note that it will idle if you close it too tightly.

* Correspondence between a holder and its adjusting knob (2) depends on the position of the syringe.

(See the figure on the left) Operate the system and notice the correspondence between the adjusting knob Nos. and the handpiece.

6 Setting/Adjustment

Maintenance panel cover (top)

6–4 Adjusting the quantity of water/air supplied to the cuspidor unit

Maintenance panel cover

Press the maintenance panel cover (top) to open it.



- (1) Water supply control knob for the syringe Adjust the quantity of water supplied to the syringe.
- (2) Air supply control knob for the syringe Adjust the quantity of air supplied to the syringe.
- (3) Water supply control knob for the water service coupler Adjust the quantity of water supplied from the water service coupler.
- (4) Bowl flush adjusting knob
- (5) Cupfiller adjusting knob*
- * Knobs (5) are provided for maintenance.

 They have already been adjusted to ensure the optimum water supply on installation.

The water level can be adjusted as required. [Reference] Setting the cupfiller water level [page 213]



All the knobs decrease the flow rate when turned clockwise and increase it when turned counterclockwise.

Do not close the adjusting knob too tightly. It is used to increase or decrease flow rate and is not a stop valve. Note that it will idle if you close it too tightly.

7-1 Exterior

7–1–1 Cleaning and disinfecting the surfaces

To clean and disinfect the exterior of the product (except the touch panel), wipe the surface with a soft cloth or paper towel moistened with FD366 manufactured by Dürr, and then wipe it with a dry cloth.

If the exterior is excessively dirty, moisten a soft cloth with water containing approx. 10% of neutral detergent, and wipe the exterior with the cloth. Then, wipe it with a cloth moistened with water and dry it completely with a dry cloth.



To clean and disinfect the touch panel, use ethanol for disinfection. Using other disinfectant may lead to incorrect operation, resulting in injury.

Never use any of the products listed below:

Volatile chemicals such as paint thinner, butanol, isopropyl alcohol, nail-varnish remover, gasoline, or kerosene; acid, alkaline or chlorine detergents; highly corrosive disinfectants (povidone-iodine such as Isodine, sodium hypochlorite, etc.); abrasive polishing wax or abrasive sponge

Do not use a brush or scrubber for maintenance. All of these may leave scratches and/or ingrained dirt.

If water or detergent is left on the surface, wipe it off immediately. Moisture or detergent may cause rust or failure of electrical parts.

Do not spray detergent directly onto the exterior.

Clean the surface with a soft cloth or paper towel moistened with detergent, and wipe it dry with a cloth.

If liquid enters the product, it may cause a malfunction or failure.

Confirm that the detergent has completely dried off before activating the product.



7-2 Chair

7–2–1 Leather part

Wipe the surface with a soft cloth or paper towel moistened with FD360 manufactured by Dürr, and then wipe it with a dry cloth.

If it is excessively dirty, moisten a soft cloth with water containing approx. 10% neutral detergent, and wipe it with the cloth. Then, wipe it with a cloth moistened with water and then dry it completely with a dry cloth.

[Reference] Precautions for use of synthetic leather [page 41]


Do not use organic solvents, detergents containing abrasives, or bleach to clean the leather part.


All of these may deteriorate the surface and change texture or gloss.


Do not spray detergent directly onto the leather part or exterior. Clean the surface with a soft cloth or paper towel moistened with detergent, and wipe it with a dry cloth.

The liquid may enter the product through gaps and cause a malfunction or failure.


Confirm that the detergent has completely dried off before activating the product.











7–3 Doctor unit

7-3-1 Touch panel

Turn off the main switch to to prevent accidental depression of a switch during cleaning or disinfection.

When cleaning or disinfection while powering on the main switch, lock the touch panel of the doctor unit.

(Example) Cleaning the surface of the touch panel during the procedure.

1. Open the [Lock mode] screen, and press OK

The touch panel is locked.

While it is locked, a sub-window indicating the locked state is displayed on the touch panel.

- 2. Wipe the touch panel with a soft cloth moistened with detergent.
- 3. Press and hold the membrane chair/headrest switch of for one second or more.

This will unlock the touch panel operation.

Do not spray detergent directly onto the exterior.

Clean the surface with a soft cloth or paper towel moistened with detergent, and wipe it with a dry cloth.

If liquid enters the product, it may cause a malfunction or failure.



Be certain to wipe off all water and detergent. Otherwise, it may cause operational failure, malfunction, resulting in injury.

7–3–2 Silicone mat/Handpiece rest

Autoclave them at a temperature of 134°C for 3 minutes. Or, wipe off the surface with soft cloth moistened with disinfectant FD366 manufactured by Dürr.

Before sterilization, remove dirt on the surface and wash them under running water.

Be sure to put them in a sterilization bag during the autoclave process.

Do not perform the drying process and dry naturally.


Repeating autoclave sterilization may cause degradation or discoloration, but doesn't affect the product functions.

If chemical solutions are spilled on the equipment, immediately wipe them off. Otherwise, discoloration may occur.

Holder type



Handle cover





7-3-3 Handle cover

Handle cover is detachable for cleaning.

Wipe it well with a soft cloth moistened with FD366 manufactured by Dürr. Handle cover can be autoclaved at a temperature of 134°C for 3 minutes.

Before sterilization, remove dirt on the surface and wash it under running water. Be sure to put it in a sterilization bag during the sterilization process.

Do not perform the drying process exceeding the sterilization temperature and dry naturally.


[Method to detach] Holder type

- ① Firstly, remove the uneven part at the edge of handle cover.
- 2 Remove the handle cover.
- * Be sure to remove it by hands.

[Method to reattach]

Reattach it in the reverse order of detaching procedures.

* Align the uneven part of the handle cover and then reattach it.



[Method to detach] Rod type

Remove the handle cover.

* Be sure to remove it by hands.

[Method to reattach]

Reattach it in the reverse order of detaching procedures.

* Align the uneven part of the handle cover and then reattach it.

Repeating autoclave sterilization may cause degradation or discoloration, but doesn't affect the product functions.

Do not perform the drying process exceeding the sterilization temperature and dry naturally.

Otherwise, deformation or discoloration may occur.

If chemical solutions are spilled on the equipment, immediately wipe them off. Otherwise, discoloration may occur



7–3–4 Waste container holder

When the waste container becomes full, replace a paper cup for the waste container holder.

It the holder becomes dirty, wipe it well with a soft cloth moistened with FD366 manufactured by Dürr.

Holder



Place holder



7–3–5 Instrument holder

Wipe the surface with a soft cloth or paper towel moistened with FD366 manufactured by Dürr, and then wipe it with a dry cloth.

If the exterior is excessively dirty, moisten a soft cloth with water containing approx. 10% neutral detergent, and wipe the exterior with the cloth. Then, wipe it with a cloth moistened with water and then dry it completely with a dry cloth.

Never use any of the products listed below:

Volatile chemicals such as paint thinners, butanol, isopropyl alcohol, nail-varnish remover, gasoline, or kerosene; acid, alkaline, or chlorine detergents; highly-corrosive disinfectants (povidone-iodine such as Isodine, sodium hypochlorite, etc.); abrasive polishing wax, or abrasive sponge


Do not use a brush or scrubber during maintenance. All of these may leave scratches and/or ingrained dirt.

If water or detergent is left on the surface, wipe it off immediately. Moisture or detergent may cause rust or failure of electrical parts.


Do not spray detergent directly onto the leather part or exterior. Clean the surface with a soft cloth or paper towel moistened with detergent, and wipe it with a dry cloth.


If liquid may enter the product through gaps and cause a malfunction or failure.

Confirm that the detergent has completely evaporated before activating the product.











Holder sleeve

The holder sleeves of the instrument holder are detachable for cleaning. Wipe it well with a soft cloth moistened with FD366 manufactured by Dürr. Sleeve No. A1 to A3 can be autoclaved at a temperature of 134°C for 3 minutes. Sleeve No.1 to 4 cannot be autoclaved.

Before sterilization, remove dirt on the surface and wash it under running water. Be sure to put it in a sterilization bag during the sterilization process.

Do not perform the drying process exceeding the sterilization temperature and dry naturally.

Regarding the sleeve No. of each handpiece / syringe, refer to the table on the next page.

[Method to detach/reattach it]

- 1. Pull the lever at the lower section of the holder sleeve toward you (1).
- 2. While pulling the lever, push the holder sleeve upward to remove it (2).
- 3. To reattach it, insert it from upper side until it 'clicks' in (3).

Each holder sleeve has its No. on the bottom, and a sticker showing the same No. is attached to the instrument holder. Make sure you attach the holder sleeve to the holder with the same No.

Make sure you attach the holder sleeves to the holders with the corresponding Nos. (to the original positions) until they 'click' in.

A mismatched combination will stop the product from functioning correctly.

Do not autoclave the sleeve No. 1 to 4.

Autoclave sterilization may deform or degrade them.

Sleeve No. A1 to A3 can be autoclaved at a temperature of 134°C for 3 minutes.

Repeating autoclave sterilization may cause degradation or discoloration, but doesn't affect the product functions.

Do not perform the drying process exceeding the sterilization temperature and dry naturally.

Otherwise, deformation or discoloration may occur.

If chemical solutions are spilled on the equipment, immediately wipe them off. Otherwise, discoloration may occur.

Non-sterile type

Sleeve No.	Applicable handpiece/syringe	
1	Syringe	BT14 3WAY LUZZANI 3WAY (Minilight) LUZZANI 6WAY (Minilight)
2	Syringe Air turbine Air motor Ultrasonic scaler	SYR-20 3WAY 77-type 3WAY LUZZANI 3WAY (Minimate) Air turbine Air motor NSK VARIOS VS170 SCALER
3	Micromotor Ultrasonic scaler Curing light	NSK NBX NSK NLX plus NSK NLX nano BIEN AIR MX2 (DMX3) BIEN AIR MCX SATELEC Xinetic SATELEC SP4055 NEWTRON EMS NO PAIN SATELEC MINI LED STD OEM
4	Syringe Ultrasonic scaler	DCI 3439 3WAY NSK VARIOS VS170 LUX SCALER DENTSPLY CAVITRON SCALER (TYPE G139) SATELEC SP4055 NEWTRON SLIM

Sterilizable type


Sleeve No.	Applicable handpiece/syringe		
A1	Syringe Air turbine	SYR-20 3WAY 77-type 3WAY Air turbine	
	Air motor	Air motor	
A2	Syringe Micromotor Ultrasonic scaler Curing light	BT14 3WAY LUZZANI 3WAY (Minilight) LUZZANI 6WAY (Minilight) BIEN AIR MCX BIEN AIR MX2 (DMX3) NSK NBX NSK NLX plus NSK NLX pano NSK VARIOS VS170 SCALER NSK VARIOS VS170 LUX SCALER SATELEC Xinetic SATELEC SP4055 NEWTRON EMS NO PAIN SATELEC MINI LED STD OEM	
A3	Syringe	DCI 3439 3WAY	
	Ultrasonic scaler	LUZZANI 3WAY (Minimate) DENTSPLY CAVITRON SCALER (TYPE G139) SATELEC SP4055 NEWTRON SLIM	



Upper part of the place holder is detachable for cleaning.



- 1. Hold the upper part of the place holder with both hands and pull it upward slightly. (1)
- 2. Pull it toward you and remove it. (2)
- 3. To reattach it, insert it to the original position from the upper side. (3)





7-3-6 BT14 3WAY syringe

Washing and sterilizing the nozzle

Nozzle of BT14 is detachable and suitable for cleaning and autoclave sterilization.

[Cleaning inside the nozzle]

Insert the accompanied nozzle cleaning tool from the tip of the nozzle. Clean the inside of the nozzle and remove the residues by spraying water and air.

If the nozzle is autoclaved with residues remained, the residues are clogged inside the nozzle, and water may not come out.

[Detaching procedure]

Pull the nozzle detaching lever to unlock the nozzle, then the nozzle is detachable.

[Washing procedure]

Wash the nozzle in the following procedures.

- 1. Wash the nozzle carefully under running water. Run the water through inside the nozzle.
- 2. Immerse the nozzle in the disinfectant ID212 manufactured by Dürr diluted with water about 25 times, and perform ultrasonic cleaning for 10 minutes or more.

Immerse the inside surface of the nozzle to the solution.

Autoclave them at a temperature of 134°C for 3 minutes.

Be sure to put them in a sterilization bag during the autoclave process.

2. Release the nozzle detaching lever and pull the nozzle a little.

3. After the ultrasonic cleaning, wash the nozzle carefully under running water again.

Run the water through inside the nozzle.

[Sterilization procedure]

[Attaching procedures]

shown in the left figure.

It clicks and locked.

when pulling it.

Attaching procedures

(b) Detaching part

Detaching procedure

(a) Nozzle detaching lever



Example of attaching nozzle Good example

Nozzle detaching lever is returned. *(a) and (b) are on the same plane



<u>^</u> \

Follow the example of attaching nozzle shown in the left figure, and check the nozzle is securely attached.

3. After the nozzle is attached, confirm that the nozzle cannot be detached

1. Pull the nozzle detaching lever and insert the nozzle until the line is invisible

WARNING

If BT14 is used with its nozzle not securely attached, it may burst out when spraying water or air, and may harm users or other people. Confirm that the nozzle is securely attached before its use.



CAUTION

Be careful not to injure yourself when using the nozzle cleaning tool because the tip of them are sharp.

Bad example



Nozzle detaching lever is not returned.

Only the nozzle can be autoclaved.

For infection control, autoclave sterilization is recommended between treatments.

Do not sterilize the nozzle except for autoclave sterilization. Autoclave sterilizer in compliance with Class B is recommended.

The temperature of autoclave sterilizer must be at 135°C or less, not exceeding 135°C. Do not perform the drying process and dry naturally if the temperature is to exceed 135°C.

If chemicals or foreign substances adhere to the nozzle, failure may result or discoloration may occur. Therefore, cleaning and washing must be done before autoclave sterilization.

The handpieces can be autoclaved up to 250 times.

For cleaning, do not insert the interdental toothbrush or the like into the nozzle inserting port while the nozzle is detached. O-ring (seal material) is attached inside the nozzle inserting port. If it's damaged, water leak may occur



Applying vaseline to the nozzle

Repeated detachment of the nozzle decreases the amount of grease for O-ring, which may stiffen the operation of detachment. If the operation of detaching nozzle stiffens, apply a little of vaseline on the surface of nozzle inserting part shown in the left figure.

Flushing

When flushing the retained water, accompanied clip for flushing (hereinafter, 'clip') is used for keeping water discharging.

When inserting the BT14 syringe inside the built-in flushing sleeve, the clip is not needed.



[Method to use]

- 1. Direct the nozzle toward the cuspidor bowl, and press the W lever and discharge water. (1)
- 2. While discharging water, insert the clip between the body and lever as shown in the left figure (2) to keep the W lever pressed.
- 3. Also perform the flushing for other handpieces equipped with the unit.
- 4. After flushing, remove the clip by pressing the W lever, and return the syringe to the instrument holder. Keep the clip safe not to lose it.




CAUTION

Be careful not to injure yourself when using the clip for flushing because the tip of them are sharp.







7-3-7 SYR-20 3WAY syringe

Cleaning the inside of the lever

If dust or dirt accumulates inside the lever, use a cotton swab to remove them.

Wash and sterilization the nozzle

Wash and sterilize the handpieces between patients.

To properly sterilize the 3way syringe, it is necessary to wash them to remove dirt and immerse them in detergent.

Then, rinse them to remove any remaining detergent.

Follow the procedure below to wash and sterilize the nozzle.

Disassembly

To prepare for washing, disassemble the nozzle as shown in the figure. Pull the ① nozzle detaching lever to unlock the nozzle, ② then the nozzle is detachable.

Washing the surface [Hand washing]

Wipe off the surface contamination by a cloth while rinsing the surface by running clean warm water at 40±5 degrees.

Scrub the tip and joint part of nozzle by a cleaning brush or by a tooth brush with running clean warm water at 40±5 degrees.

Check whether contamination is removed or not after cleaning. Continue the cleaning if contamination is remained.

Immersed with an alkaline disinfection or detergent for 5 minutes. (We recommend to use ID212 made by Dürr)

Rinse thoroughly by distilled water at ordinary temperature or by clean water for more than 1 minute.

[Hand washing/Ultrasonic bath]

Clean nozzle under running water for 30 seconds with a soft brush and place in an ultrasonic bath with an enzymatic cleaner to remove superficial debris prior to sterilization.

If debris remains, the nozzle will not be properly sterilized.



CAUTION


Wash the nozzles immediately after use.

If chemicals or foreign substances adhere to the nozzle, failure may result or discoloration may occur.

Therefore, cleaning and washing must be done before autoclave sterilization. If the dirt cannot be removed, replace the nozzles.

The nozzle can be autoclaved up to 250 times.

Disassembly



Washing the surface




Sterilization



Attaching the nozzle


Nozzle detaching lever




line is invisible.




Example of attaching nozzle Good example







Bad example



Sterilization

Choose the appropriate method from the following sterilization cycles depending on the type of the autoclave sterilizer in your clinic:

[Dynamic-Air-Removal]

- 1. Put the nozzle in a sterilization bag, and seal the opening.
- 2. Autoclave it at a temperature of 134°C for 3 minutes with a 15-minute drying time.

[Gravity displacement]

- 1. Put the nozzle in a sterilization bag, and seal the opening.
- 2. Autoclave it at a temperature of 132°C for 15 minutes with a 30-minute drying time.



CAUTION

Sterilization must be done every after use to patients.

Do not sterilize the nozzle except for autoclave sterilization.

Autoclave sterilizer in compliance with Class B is recommended.

Sterilization temperature is 135°C or less.

Do not perform the drying process and dry naturally if the temperature for drying process is to exceed 135°C.

If damage occurs to the sterilization bag, discard and sterilize again using a new sterilization bag.

Storage method

After sterilization, store the nozzle in the sterilization bag in a dark, cool place.

Attaching the nozzle

Pull the ① nozzle detaching lever and insert the nozzle until ② the black line is invisible shown in the left figure.

Release the nozzle detaching lever and 3 pull the nozzle a little.

It clicks and locked.

After the nozzle is attached, confirm that the nozzle cannot be detached when pulling it.


Follow the example of attaching nozzle shown in the figure, and check the nozzle is securely attached.



WARNING

If SYR-20 3way syringe is used with its nozzle not securely attached, it may burst out when spraying water or air, and may harm users or other people.

Confirm that the nozzle is securely attached before its use.



Disassembly



7-3-8 77-type 3WAY syringe

Disassembly

To prepare for washing, disassemble the nozzle as shown in the figure. Pull the 1 nozzle detaching lever to unlock the nozzle, 2 then the nozzle is detachable.

Washing

Hand washing

Wipe off the surface contamination by a cloth while rinsing the surface by running clean warm water at 40±5 degrees.

Scrub the tip and joint part of nozzle by a cleaning brush or by a tooth brush with running clean warm water at 40 ± 5 degrees.

Check whether contamination is removed or not after cleaning.

Continue the cleaning if contamination is remained.

Immersed with an alkaline disinfection or detergent for 5 minutes.

(We recommend to use ID212 made by Dürr)

Rinse thoroughly by distilled water at ordinary temperature or by clean water for more than 1 minute.

Hand washing/Ultrasonic bath

Clean nozzle under running water for 30 seconds with a soft brush and place in an ultrasonic bath with an enzymatic cleaner to remove superficial debris prior to sterilization.

If debris remains, the nozzle will not be properly sterilized.



CAUTION

Cleaning must be done every after use to patients.

Wash the nozzles immediately after use.

If chemicals or foreign substances adhere to the nozzle, failure may result or discoloration may occur. Therefore, cleaning and washing must be done before autoclave sterilization.

If the dirt cannot be removed, replace the nozzles.

The handpieces can be autoclaved up to 250 times.

Sterilization

Choose the appropriate method from the following sterilization cycles depending on the type of the autoclave sterilizer in your clinic:

[Dynamic-Air-Removal]

- 1. Insert the nozzle in a sterilization bag and seal it.
- 2. Autoclave them at a temperature of 134°C for 3 minutes with a 15-minute drying time.

[Gravity displacement]

- 1. Insert the nozzle in a sterilization bag and seal it.
- 2. Autoclave them at a temperature of 132°C for 15 minutes with a 30-minute drying time.



CAUTION


Sterilization must be done every after use to patients.


Sterilization by class B cycles.

Sterilization temperature is 135°C or less.

Do not perform the drying process and dry naturally if the temperature is to exceed 135°C.


If damage occurs to the sterilization pouch, discard and sterilize again using a new pouch.







Attaching the nozzle

Example of attaching nozzle Good example





Bad example



Storage

After sterilizing the nozzle, keep it in the sterilization pouch and store in a dark and cool place.

Attaching the nozzle

Pull the ① nozzle detaching lever and insert the nozzle until ② the black line is invisible shown in the left figure.

Release the nozzle detaching lever and pull the nozzle a little.

It clicks and locked.


After the nozzle is attached, confirm that the nozzle cannot be detached when pulling it.

Follow the example of attaching nozzle shown in the figure, and check the nozzle is securely attached.



WARNING

If 77 type 3way syringe is used with its nozzle not securely attached, it may burst out when spraying water or air, and may harm users or other people. Confirm that the nozzle is securely attached before its use.

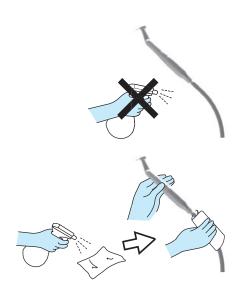

7–3–9 Handpiece hose


When the handpiece becomes dirty, wipe it well with a soft cloth moistened with FD366 manufactured by Dürr.

Do not spray detergent directly onto the exterior.

Clean the surface with a soft cloth or paper towel moistened with detergent, and wipe it with a dry cloth.

If liquid enters the product, it may cause a malfunction or failure.

Confirm that the detergent has completely evaporated before activating the product.



7–3–10 Oil mist separator


This unit collects oil from the exhaust air from the handpiece.

When oil reaches to the line on the oil reservoir (1), make sure you discard the oil.

Turn the oil reservoir counterclockwise to remove.

If the hygroscopic sponge (2) (consumable) is excessively dirty or has excessive oil on it, replace it.

Contact your local authorized Belmont dealer for a replacement for the hygroscopic sponge. (Replacement will be charged for.)



7–4 Cuspidor unit

7-4-1 Assistant holder

Wipe the surface with a soft cloth or paper towel moistened with FD366 manufactured by Dürr, and then wipe it with a dry cloth.

If the exterior is excessively dirty, moisten a soft cloth with water containing approx. 10% neutral detergent, and wipe the exterior with the cloth. Then, wipe it with a cloth moistened with water and then dry it completely with a dry cloth.

Never use any of the products listed below:

Volatile chemicals such as paint thinners, butanol, isopropyl alcohol, nail-varnish remover, gasoline, or kerosene; acid, alkaline, or chlorine detergents; highly-corrosive disinfectants (povidone-iodine such as Isodine, sodium hypochlorite, etc.); abrasive polishing wax or abrasive sponge.

Do not use a brush or scrubber during maintenance. All of these may leave scratches and/or ingrained dirt.


If water or detergent is left on the surface, immediately wipe it off. Any remaining moisture or detergent may cause rust or failure of electric parts.

Do not spray detergent directly onto the exterior.

Clean the surface with a soft cloth or paper towel moistened with detergent, and wipe it with a dry cloth.

If liquid enters the product, it may cause a malfunction or failure.

Confirm that the detergent has completely evaporated before activating the product.



The holder sleeves of the instrument holder are detachable for cleaning. Wipe it well with a soft cloth moistened with FD366 manufactured by Dürr. Sleeve No. A1 to A4 can be autoclaved at a temperature of 134°C for 3 minutes. Sleeve No.1 to 6 cannot be autoclaved.


Before sterilization, remove dirt on the surface and wash it under running water. Be sure to put it in a sterilization bag during the sterilization process.

Do not perform the drying process exceeding the sterilization temperature and dry naturally.


Regarding the sleeve No. of each handpiece / syringe, refer to the table on the next page.


[Method to detach/reattach it]

- 1. Pull the lever at the lower section of the holder sleeve toward you (1).
- 2. While pulling the lever, push the holder sleeve upward to remove it (2).
- 3. To reattach it, insert it from upper side until it 'clicks' in (3).



Assistant holder







Each holder sleeve has its No. on the bottom, and a sticker showing the same No. is attached to the assistant holder.

Make sure you attach the holder sleeve to the holder with the same No.

Make sure you attach the holder sleeves to the holders with the corresponding Nos. (to the original positions) until they 'click' in.

A mismatched combination will stop the product from functioning correctly.

Do not autoclave the sleeve No. 1 to 6.

Autoclave sterilization may deform or discolor them.

Sleeve No. A1 to A4 can be autoclaved at a temperature of 134°C for 3 minutes.

Repeating autoclave sterilization may cause degradation or discoloration, but doesn't affect the product functions.

Do not perform the drying process exceeding the sterilization temperature and dry naturally.

Otherwise, deformation or discoloration may occur.


If chemical solutions are spilled on the equipment, immediately wipe them off. Otherwise, discoloration may occur.


Non-sterile type

Sleeve No.	Applicable handpiece/syringe	
1	Syringe	BT14 3WAY
		LUZZANI 3WAY (Minilight)
		LUZZANI 6WAY (Minilight)
2	Syringe	SYR-20 3WAY
		77-type 3WAY
		LUZZANI 3WAY (Minimate)
3	Curing light	SATELEC MINI LED STD OEM
4	Syringe	DCI 3439 3WAY
	Saliva ejector handpiece	Dürr
5	Vacuum handpiece	VH-18
		Dürr
6	Saliva ejector handpiece	BT06

Sterilizable type

Sleeve No.	Applicable handpiece/syringe	
A1	Syringe	SYR-20 3WAY
		77-type 3WAY
A2	Syringe	BT14 3WAY
		LUZZANI 3WAY (Minilight)
		LUZZANI 6WAY (Minilight)
	Curing light	SATELEC MINI LED STD OEM
A3	Syringe	DCI 3439 3WAY
		LUZZANI 3WAY (Minimate)
	Saliva ejector handpiece	Dürr
A4	Vacuum handpiece	VH-18
		Dürr





7–4–2 Assistant hose clamp

Assistant hose clamp of the assistant unit is detachable from the frame, which is suitable for cleaning.

When it becomes dirty, wipe it well with a soft cloth moistened with FD366 manufactured by Dürr.

[Method to detach]

- (1) Remove the assistant hose clamp from the frame.
 - * Be sure to remove it by hands.
- (2) Remove the hose from the assistant hose clamp.


[Method to reattach]

Reattach it in the reverse order of detaching procedures.

Do not autoclave them.

Autoclave sterilization may deform or discolor them.





7-4-3 Assistant silicone mat

Autoclave them at a temperature of 134°C for 3 minutes. Or, wipe off the surface with soft cloth moistened with disinfectant FD366 manufactured by Dürr.


Before sterilization, remove dirt on the surface and wash them under running water.

Be sure to put them in a sterilization bag during the autoclave process.

Do not perform the drying process and dry naturally.

Repeating autoclave sterilization may cause degradation or discoloration, but doesn't affect the product functions.

If chemical solutions are spilled on the equipment, immediately wipe them off. Otherwise, discoloration may occur.

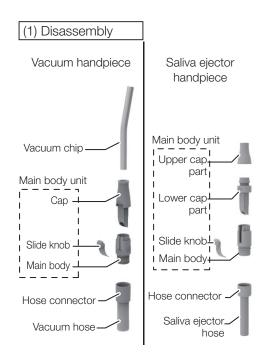

(2) Washing the surface




(3) Washing the interior and sliding part

Scrubbing brush or toothbrush



Sliding groove

(4) Washing parts inaccessible with a brush



7–4–4 Washing and sterilizing the vacuum handpiece and saliva ejector handpiece

Wash and sterilize the handpieces between patients.

To properly sterilize the vacuum and saliva ejector handpieces, it is necessary to wash them to remove dirt and immerse them in detergent.

Then, rinse them to remove any remaining detergent.

Follow the procedure below to wash and sterilize the handpieces.

(1) Disassembly

To prepare for washing, disassemble the handpieces as shown in the figure. Hold the hose connector, and pull the vacuum hose and saliva ejector hose to detach them from the main body.

(2) Washing the surface

Rinse the surface with clean water (tap water) warmed to a temperature of 40 \pm 5°C, and rub it with a cloth to remove dirt. When all dirt is removed, wipe it dry.

(3) Washing the interior and sliding groove

Rinse the interior and sliding groove of the main body with clean water (tap water) warmed to a temperature of $40 \pm 5^{\circ}$ C, and scrub them with a scrubbing brush or toothbrush. When all dirt is removed, wipe them dry.

(4) Washing parts inaccessible with a brush

If some parts are inaccessible with a brush, rub them with a cloth.

Rinse them well with clean water (tap water) warmed to a temperature of 40 \pm 5°C (for at least 1 minute).

Immerse the parts in ID212 manufactured by Dürr or alkaline cleaner for 5 minutes. Then, rinse them well with clean water (tap water) warmed to a temperature of $40 \pm 5^{\circ}$ C (for at least 1 minute).

Inspect the parts for any visible dirt. If any visible dirt remains, repeat the above washing process.


Wash them immediately after use.


If the parts are in the condition described below after washing, do not autoclave them. Replace them.


A hole/holes are clogged, and dirt cannot be removed.

Dirt on some parts or solid dirt cannot be removed.

Caution when assembling vacuum handpiece before sterilization VH-18

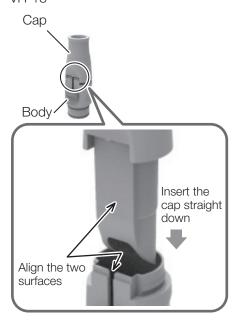

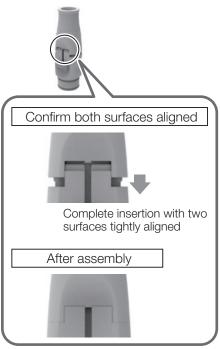



(5) Sterilization

The vacuum handpiece and saliva ejector handpiece are autoclavable. Reassemble the main body unit, and autoclave the vacuum and saliva ejector handpieces.

When assembling the vacuum handpiece, align the two surfaces; a flat surface of the cap and the surface of the sliding groove of the body. Then, slide the cap into the body straight.

- * Do not insert it twisted.
- 1. Put the handpiece in a sterilization bag, and seal the opening.
- 2. Autoclave sterilization

Sterilization temperature and sterilization time for each vacuum handpiece are as follows.

Dürr: 134°C for 5 minutes.

VH-18 / BT06: 134°C for 3 minutes.

If the temperature is to exceed 135°C during the drying process, do not perform the drying process and dry naturally.

The handpieces can be autoclaved up to 250 times.

Storage method: After sterilization, store the handpiece in the sterilization bag in a dark, cool place.





After autoclave sterilization, disassemble the handpieces, apply Vaseline, and reassembly before use.

If the handpieces are used without Vaseline, a packing may be damaged, resulting in leakages.

Vacuum handpiece



Saliva ejector handpiece




Vacuum handpiece / Saliva ejector handpiece

Suction a cup of water (approx. 100 ml) or more into the vacuum and saliva ejector handpieces after use by a patient. This is to clean and dilute the medicine used and to prevent the handpieces deteriorating.

Some medicines used for the procedure may cause deterioration of the handpiece. It may dissolve, deform, or damage part of the handpiece, possibly resulting in leaks from the handpiece or suction failure. This will ultimately makes the handpiece unusable.

Please wash them properly to ensure long-term use.

Vacuum hose / Saliva ejector hose




The exterior of the hose can be washed under tap water.

* For washing the hose interior (of the vacuum and saliva ejector lines), refer to [page 246].

To reattach the hose, insert the joint into the receptacle.

Always turn off the main switch before pulling the hose off to wash it.



[Chemical solution: Orotol plus]



7–4–5 Vacuum line / Saliva ejector line

Handpieces for vacuum and saliva ejector suction the secretions, saliva, or blood that contains bacteria. Therefore, always wash and sterilize them using chemical solution specified by us after the procedure.

[Reference] Chemical solution specified by us [page 191]
Do not use any detergent except our designated one. Otherwise, strong acidic detergents or alkaline drain preparations may cause clog, damage, or metal corrosion.

7-4-6 BT14 3WAY syringe

[Reference] BT14 3WAY syringe [page 233]

7–4–7 SYR-20 3WAY syringe

[Reference] SYR-20 3WAY syringe [page 235]

7–4–8 77-type 3WAY syringe

[Reference] 77-type 3WAY syringe [page 237]


7–4–9 Sensor window for cupfiller

Wipe the surface with a soft cloth or paper towel moistened with FD366 manufactured by Dürr, and then wipe it with a dry cloth.

If the exterior is excessively dirty, moisten a soft cloth with water containing approx. 10% neutral detergent, and wipe the exterior with the cloth. Then, wipe it with a cloth moistened with water and then dry it completely with a dry cloth.











7-4-10 Cuspidor bowl

Cuspidor bowl / Cupfiller unit

Use MD550 manufactured by Dürr as detergent for cuspidor bowl.

(1) Cuspidor bowl

The cuspidor bowl is detachable and can be washed under tap water. Lift it in the direction shown with the arrow to detach it.

After reattaching it, check that it is securely mounted before use.



CAUTION

Put on the cleaning gloves when detaching cuspidor bowl. Cuspidor bowl is made of ceramic that might cause injury when broken.

Always turn off the main switch before detaching the cuspidor bowl.

(2) Strainer (3) Drain outlet cover

Since the strainer easily gets clogged, detach the (3) drain outlet cover and clean the filter after consulting hours every day.

(4) Cupfiller base (5) Sensor window for cupfiller

Before cleaning, turn off the main switch, or switch the mode to the sensor disabled mode. [page 153]

(6) LED indicator

Wipe the LED indicator with a soft cloth moistened with FD366 manufactured by Dürr to remove dirt and water droplets.

(7) Lower section of the drain trap

If the drain trap has not been completely drained, dirt may accumulate on the inside wall. Turn the cuspidor bowl by 90 degrees as shown in the figure, turn the (7) lower section of the drain trap counterclockwise to detach, and clean it. When detaching the (7) lower section of the drain trap, dirty water may overflow from the inside. Always detach the (2) strainer and (3) drain outlet cover, and flush out the cuspidor bowl with a cup of water before detaching the (7) lower section of the drain trap. (This reduces the quantity of dirty water in the drain trap.) To reattach it, rotate the lower section of the drain trap clockwise until the vertical line meets the triangle mark.

When the lower section of the drain trap is detached, do not flush water in the cuspidor bowl.

To avoid the odor from the drain, flush the cuspidor bowl after cleaning.

Do not use sandpaper, wire wool, abrasive sponge, or abrasive cleaner.

Do not use any detergent except our designated one. Otherwise, strong acidic detergents or alkaline drain preparations may cause clog, damage, or metal corrosion.

Do not allow any metal object to come into contact with the cuspidor bowl when detaching or reattaching it since contact may leave a metal mark. If the metal object marks the bowl, use a metal mark removing agent (commercially available).

* A metal mark is a black or silver line caused by strong contact and friction between the ceramic surface and the metal object.

Before detaching or reattaching the cuspidor bowl, always turn off the main switch. When cleaning the cupfiller base, turn off the main switch, or switch the mode to the sensor disabled mode.

When detaching or reattaching the bowl, the cupfiller sensor may detect your hand or other object, causing water for flushing the bowl or cupfiller base to splash around, which can cause metal parts to rust.

The cuspidor bowl is made of ceramic. It may break if it receives a hard knock. Do not wash it with boiling water, as this may break it.

Since the cuspidor bowl can be easily detached or reattached, do not apply excessive force except when washing. (Do not knock it, hit it, or drop it.)

Do not pour water over the cupfiller base when cleaning it. It is not waterproof, and excessive water may cause it to malfunction.

For cleaning the cupfiller base, refer to the [page 247].

Do not let water flow onto the cupfiller base. The drainage function of the cupfiller base is designed to drain away any overflow water when filling a cup.

7-4-11 Solid collector

After consulting hours, remove the filter from the solid collector in the cuspidor unit, and wash it.

Accumulated debris may degrade the suction force of the vacuum handpiece or saliva ejector handpiece.

[Method to detach/reattach the filter]

1. Press the maintenance panel cover (top) of the cuspidor unit to open it.



2.



2. Pull off the solid collector.






Solid collector cap




- 3. Detach the solid collector cap from the filter.
 - Pull the filter to detach the solid collector cap as shown in the figure on the left.
- 4. Wash the solid collector cap and the filter under running water.



Wider part of the knob



Proper alignment (The wider part of the knob is located in the upper section.)



the upper section.)

- 5. Align the claw on the solid collector cap with the groove on the filter to attach them.
- 6. Attach the solid collector in its original position with the cap aligned as shown in the left figure.

Press the solid collector into the end of the receptacle with the proper alignment. If it is improperly mounted, the vacuum handpiece and saliva ejector handpiece may not function properly.

7-4-12 Spittoon valve

Clean the Spittoon valve twice in a day at the end of morning treatment and evening treatment. (At the end of evening treatment if cleaning once in a day.)




1. Press the function switch . The Function setting screen appears.



2. Press 'Spittoon valve cleaning'.

Spittoon valve cleaning screen appears.



3. Fill the spittoon bowl with chemical solution and press oκ

1 liter of diluted "Orotol Plus" is recommended for chemical solution. If you would like to use other solutions, please check with the retailer or distributor in advance.




- 4. Spittoon valve cleaning starts
 - 'Spittoon valve in cleaning' message appears on the screen.



- 5. Spittoon valve cleaning finishes
 - 'Spittoon valve in cleaning' message disappears from the screen.







7-4-13 Air filter

Empty any water that has collected in the air filter at least once a week.

- 1. Open the Junction cover.
- 2. Prepare a cup to put the water in.
- 3. Turn the drain valve knob counterclockwise, and discharge the water into the cup.
- 4. When no more water comes out, turn the drain valve knob clockwise to close it.

After closing the drain valve knob, water remained in the tube may come out. Wipe the water with cloth to prevent the water from coming out.

If any water gets into the air line, it may cause a failure of the product.

7-4-14 Air compressor

For maintenance of the air compressor, follow the Instructions for Use supplied with the air compressor.

7–4–15 Vacuum pump

For maintenance of the vacuum pump, follow the Instructions for Use supplied with the vacuum pump.

7–5 How to detach battery of the doctor unit

Instrument delivery: Holder/Place holder

 Remove the four screws under the doctor table and detach the doctor table.




2. Remove the seven screws and detach the table top.



3. Detach the button battery (CR1632) on the PCB.








Instrument delivery: Rod

1. Remove the four screws and detach the rear cover.



Rear cover

2. Detach the button battery (CR1632) on the PCB.

7-6 Maintenance and inspection

Notes on daily maintenance and inspection (by the user)

It is the responsibility of the user (medical institution) to ensure that the medical device is correctly maintained and inspected. To ensure safe use of this product, the unit must be inspected at the specified intervals as described in the table below:

No	Inspection item	Inspection interval	Inspection procedure and criteria	Outcome if inspection is not conducted	Maintenance required when the inspection criterion is not satisfied
1	Check the cancel function	Before consulting hours	When the chair is in automatic operation, it must stop when any of the operation switches shown on [page 110] is pressed or stepped on.	The chair unexpectedly moves during procedure, resulting in an injury. The patients may be caught between the doctor unit and the chair, resulting in an accident.	If the chair does not stop, please contact your local authorized Belmont dealer.
2	Check for water, air and oil leaks	Before consulting hours	Check that no water, air or oil leaks out from the product.	The product does not function properly, preventing proper treatment or procedure.	If water, air or oil leaks out, please contact your local authorized Belmont dealer.
3	Cup-filling	Before consulting hours	Place a cup on the cupfiller base, and check that the cup is detected and correctly filled. * Use a cup with a weight of 3 grams or more.	The cup is not filled with water in some cases.	Follow the description under 'Cupfiller,' and inspect it again. [page 153] If it cannot be solved after reinspection, please contact your local authorized Belmont dealer.
4	Check the functioning of each handpiece	Before consulting hours	 (1) Check that the turbine rotates properly and that the correct quantities of water and air are supplied. (2) Check that the micromotor rotates properly and that the correct quantity of water is supplied. (3) Check that the ultrasonic scaler vibrates properly and that the correct quantity of water is supplied. (4) Check that the correct quantities of water and air are supplied from syringe. 	The patient may receive an injury to their mouth, or the handpiece may malfunction.	Adjust the quantity of water or air. [page 223] For other failures, please refer to the Instructions for Use for the respective handpieces. If the problem still persists, please contact your local authorized Belmont dealer.
5	Check the functioning of lever (syringe)	Before consulting hours	Water, air, and spray come out by pressing A lever and W lever. No wobbliness is observed when pressing the lever.	The product does not function properly, preventing proper treatment or procedure.	Contact your local authorized Belmont dealer.
6	Check the correct burr for the turbine, air motor, and micromotor is mounted.	Before each patient	Check that the correct burr is securely mounted. Make sure you refer to the Instructions for Use for the turbine, air motor and micromotor. Check that the burr is free of any defect (damage or deformation).	The burr will not rotate freely, resulting in an accident.	If the burr is damaged, deformed or has some other defect, replace the burr by following the Instructions for Use for the turbine, air motor and micromotor.
7	Check the scaler tip	Before each patient	Check that the correct tip is securely mounted and properly used. Refer to the Instructions for Use for the scaler. Check that the tip is free from any defect (wear or deformation).	The tip will not vibrate properly, resulting in an accident.	If the tip is worn or deformed, replace it by following the Instructions for Use for the scaler. For other defects, please contact your local authorized Belmont dealer.

No	Inspection item	Inspection interval	Inspection procedure and criteria	Outcome if inspection is not conducted	Maintenance required when the inspection criterion is not satisfied
8	Check for the lock of the nozzle (BT14/SYR- 20/77-type)	Before each patient	Check that the nozzle is securely locked. Check that the locked nozzle does not detach when pulling it.	The nozzle may burst out and harm users or other people.	Securely lock the nozzle. [pages 233, 236 and 238] When any malfunction is observed, please contact your local authorized Belmont dealer.
9	Debris on the micromotor	After consulting hours	Check that no excess oil from the handpiece adheres to the motor unit.	The motor unit may not function properly, resulting in a malfunction.	Follow the Instructions for Use for the micromotor to maintain it.
10	Maintenance Vacuum handpiece / saliva ejector handpiece	After consulting hours	Wash the vacuum lines and saliva ejector lines.	Suction is defective.	Wash the vacuum lines. [page 246]
11	Maintenance Cuspidor bowl	After consulting hours	Check that the cuspidor bowl does not contain any dirt (or excrescence). Check that no dirt has collected on the dirt filter.	Draining is defective.	Clean the cuspidor bowl and dirt filter. [pages 247, 248]
12	Maintenance Solid collector	After consulting hours	Check that no dirt has collected on the solid collector.	Suction power of the vacuum handpiece or saliva ejector handpiece has decreased.	Clean the filter. [page 249]
13	Maintenance Exterior	After consulting hours	Check that no chemical solution or dirty water adheres to or remains on the exterior of the product.	Any liquid remaining will causes discoloration or change the properties of the exterior or cause metal parts to rust.	Clean it. [page 225]
14	Check the main switch and main water valve	After consulting hours	Check that the main switch is turned off, and the main water valve is closed.	May result in a short circuit or water leaks.	If the main switch cannot be turned off or the main water valve cannot be closed, please contact your local authorized Belmont dealer.
15	Movable parts of the product	Once a week	When operating the product, check that no movable parts emit any abnormal noise.	The product does not function properly, preventing proper treatment or procedure.	If any movable parts emit an abnormal noise, please contact your local authorized Belmont dealer.
16	Maintenance Drain valve	Once a week	Drain water from the drain valve on the air filter.	Water enters the air line, resulting in a malfunction.	Always drain the air filter. [page 251]
17	Check water and pneumatic pressures	Once a month	Check the water and pneumatic pressures using the pressure gauge on the maintenance panel. Main water pressure: 0.2 MPa Main air pressure: 0.5 MPa	The product does not function properly, preventing proper treatment or procedure.	If the pressure is out of the range of the main water pressure/main air pressure, please contact your local authorized Belmont dealer.
18	Check the doctor unit	Once a month	The doctor table is level and stops at the specified position.	Objects fall from the doctor table, resulting in an injury or accident.	If the doctor table is not level or does not stop at the specified position, please contact your local authorized Belmont dealer.
19	Oil mist separator	Once a month	The drain oil does not reach the line on the oil mist separator.	The handpiece may not function properly due to an exhaust failure.	Empty the oil. [page 239]



Always refer to this Guide and the Instructions for Use supplied with each device (such as the dental light and handpieces) before conducting daily maintenance and inspection.

If you do not conduct daily maintenance or inspection, use of the product may result in injury or damage to nearby devices.

Notes for periodic inspection

The product contains parts that stop functioning or wear depending on the use frequency, and therefore it is important to carry out maintenance in a periodic inspection once a year (including replacement of consumables) and safety checks.

Service parts required for the periodic inspection (including consumables) are listed in the table below. However, depending on the specifications of your device, there may be alternative parts available that differ from those listed in the table below.

Maintenance and inspection can be outsourced to qualified persons such as authorized repairers of medical devices.

If you have any question about periodic inspection, contact your local authorized Belmont dealer.

List of service parts required for the periodic inspection

Part name	Standard service life	Part name	Standard service life
Movable part	7 years	Switch	5 years
Wire for a movable part	5 years	PC board	5 years

List of consumables required for periodic inspection

Part name	Part name	
O-ring	Diaphragm	
Packing	Saliva ejector nozzle	



WARNING

Always entrust periodic inspection to your local authorized Belmont dealer. If you do not carry out periodic inspection, use of the product may cause injury or damage to nearby devices.

7–7 Detachable parts

Part name	Part name
Handpiece	Vacuum tip
Handpiece hose	Saliva ejector nozzle
Holder sleeve	Solid collector cap
Cuspidor bowl	Solid collector filter
Cover for the drain outlet of the cuspidor bowl	Water service coupler
Cuspidor bowl strainer	Air service coupler
Vacuum handpiece	Syringe nozzle
Saliva ejector handpiece	Syringe body
Oil mist separator	Syringe hose

7–8 Storage method

If the product is not used for an extended period of time after consulting hours or during holidays, make sure you observe the precautions below:

- Always turn off the main switch after consulting hours.
 (This is to stop supply of air, water, and electric power.)
 Make it a habit to do this to prevent water leak and electrical accidents.
- 2. After consulting hours, turn the water main valve knob counterclockwise to the vertical position to close the water main valve. Make it a habit to do this to prevent accidents by water leaks.
- 3. Turn off the breaker for the compressor, and discharge air. (Also make sure you have turned off the power.)
- 4. Turn off the breaker for the vacuum pump. (Also make sure you have turned off the power.)
- 5. Turn off the breaker for the device in the clinic. (Also make sure you have turned off the power.)
- 6. Set the chair to the lowest position and the backrest to the most reclined position.

8 Maintenance by Service Engineers

8–1 After-sales service

When you request for repair

Refer to 'Troubleshooting' [from page 259 on] before you check the device. If the problem persists, turn off the main switch, and contact your local authorized Belmont dealer to request a repair.

8-2 Service life

The service life of this product is 10 years on condition that maintenance and inspection are properly conducted [according to our self-certification (our data)]. However, the standard service lives of service parts that require periodic inspection vary according to the part. [page 256]

8-3 Period of Parts Retention

We hold service parts such as consumables for products for 10 years from the time of launch.

* Service parts are parts required for repair to return the product to the original state and functions or to maintain its functions.

9-1 Troubleshooting

If you encounter any of the problems listed below, take the countermeasures described below before requesting a repair. If the problem persists even after troubleshooting, stop using the product immediately, turn off the main switch, and contact your local authorized Belmont dealer.

Phenomenon	Please check	Remedy
The product does not work at all.	Is the main switch turned on?	Turn on the main switch. [page 63]
	Is the power to the compressor turned on?	Turn on the power.
	Is the breaker for the device on the switchboard of the dentist's office turned on?	Turn on the breaker for the device.
The chair does not move.	Is the chair lock function activated?	Unlock the chair. [pages 111 to 114]
	Have you been operating the product continuously for a long time?	The overheating prevention device for the hydraulic motor has been triggered. Wait for approx. 10 minutes, and move the chair.
The product cannot be operated with the wireless foot controller.	Are the correct batteries inserted?	Insert the batteries with proper polarities. [page 148]
	Are the batteries flat?	Replace the batteries with new (or charged) ones with proper polarities. [page 148]
	Is the wireless foot controller too far away from the product?	Keep the distance between the foot controller and product to approx. 1 meter or less.
	If you are using more than one products, are you mixing it up with another product's foot controller?	Check the pairing identification code, and use the combination with the same codes. [page 147]
No air is being supplied.	Is the power to the compressor turned on?	Turn on the power.
	Is the knob that controls the air supply to the syringe or other parts closed?	Open the air supply control knob. [pages 223, 224]
No water is being supplied.	Is the water main valve closed?	Open the water main valve. [page 62]
	Is the water supply control knob to the handpiece or syringe closed?	Open the water supply control knob. [pages 223, 224]
The vacuum handpiece or saliva ejector	Is the power to the vacuum pump turned on?	Turn on the power.
handpiece does not activate the suction function.	Is the solid collector filter dirty?	Clean the filter. [page 249]
	Is the solid collector filter properly attached?	Attach the solid collector properly. [page 249]
Is there a message displayed on the touch panel?	Read the message.	Take the corrective measures indicated in the message. [pages 260 to 262]
Water keeps running from the cupfiller and doesn't stop.	Is there any dirt or droplet on the surface of cupfiller sensor?	Turn off the main switch and clean the surface of the cupfiller sensor.
Water doesn't come out of the cupfiller.	Is there any dirt or droplet on the surface of cupfiller sensor?	Turn off the main switch and clean the surface of the cupfiller sensor.
	Isn't the sensor disable mode activated?	Cancel the sensor disable mode. [page 153]

9–2 Message on the touch panel and measures to be taken

Phenomenon	Please check	Remedy
E01: Communication w/cuspidor section	Internal communication error for the device	Turn off the main switch, and contact your local authorized Belmont dealer.
E02: Communication w/FC		
E03: Communication w/water heater (HP)		
E04: Communication w/micromotor		
E05: Communication w/scalar		
E06: Communication w/chair		
E07: Communication w/cupfiller		
E08: Communication w/Washing the vacuum line		
E12: Control panel (Dr.)	The membrane switch is pressed when the power is turned on.	Keep your hand away from the membrane switch. If the error code does not go off when your hand is removed, contact your local authorized Belmont dealer.
E13: Control panel (ASST)	The switch on the assistant's control panel is pressed when the power is turned on.	Keep your hand away from the assistant's control panel. If the error code does not go off when your hand is removed, contact your local authorized Belmont dealer.
E14: Air pressure too low	The master pressure in the pneumatic system decreases.	Turn off the main switch, and contact your local authorized Belmont dealer.
E20: HP picked up while FC is on	The pedal of the foot controller is stepped on when the handpiece is picked up.	Release the pedal of the foot controller. If the error code does not go off when you take your foot off, contact your local authorized Belmont dealer.
E22: Foot controller (Slide)	A wire in the foot controller has become disconnected.	Turn off the main switch, and contact your local authorized Belmont dealer.
E24: Communication line with FC is busy.	Communications from the foot controller are jammed. (Wireless foot controller)	Use the cable contained in the package.
E25: Foot controller EEPROM	EEPROM (memory contents) read error for the foot controller	Turn off the main switch, and contact your local authorized Belmont dealer.
E30: Chair EEPROM	EEPROM (memory contents) read error for the chair	
E31: Potentiometer (Seat)	Chair position detection error	
E32: Potentiometer (Backrest)		
E34: Thermistor (Solenoid valve)	Chair oil temperature detection error	

Message on the touch panel	Details	Remedy
E35: Stick switch	The stick switch is pressed when the power is turned on.	Check that there is not a leg or an object in contact with the stick switch on the chair. If nothing is in contact with it but the error code does not go off, contact your local authorized Belmont dealer.
E38: Potentiometer (Headrest)	Chair position detection error	Turn off the main switch, and contact your
E39: Timeout (Chair)	In automatic operation, the chair cannot complete the movement to the target position within the specified time.	local authorized Belmont dealer.
E42: Timeout (Cupfiller)	Cup-filling was not completed within the specified time.	If the water supply is insufficient, adjust the supply with the cupfiller control knob. If the error code does not go off after adjustment, contact your local authorized Belmont dealer.
E43: Cupfiller EEPROM	EEPROM (memory contents) read error in cupfiller	Turn off the main switch, and contact your local authorized Belmont dealer.
E44: No water in the bottle	The water level detection inside the bottle or the solenoid valve is behaving abnormally.	Press the switch. Return the vacuum and saliva ejector handpieces to the instrument holder, and then contact your local authorized Belmont dealer.
E45: Water in the bottle cannot be discharged.	The vacuum and saliva ejector handpiece are not connected to the insertion point.	Press the OK switch and try again.
	The water level detection inside the bottle or the water suctioning function is behaving abnormally.	Press the switch. Return the vacuum and saliva ejector handpieces to the instrument holder, and then contact your
E46: Cleaner pump is not functioning.	The pump is overloaded.	local authorized Belmont dealer.

Message on the touch panel	Details	Remedy	
C01: Cancelled. Dr table is in the way.	The doctor table has been moved behind the backrest while the chair is moving, and the chair stops in the middle.	Move the doctor table next to the armrest, and move the chair.	
C02: Cancelled. Dr table is in contact.	An object is interfering with the doctor table while the chair is moving, and the chair stops in the middle.	Remove the cause of the emergency stop, and move the chair. When the chair moves properly, the error code will go off.	
C03: Cancelled. Asst arm is in contact.	An object is interfering with the assistant arm while the chair is moving, and the chair stops in the middle.		
C04: Cancelled. Cuspidor bowl is in the way.	The cuspidor bowl is removed while the chair is moving, and the chair stops in the middle.	Return the cuspidor bowl, and move the chair.	
C05: Cancelled. Footrest is in contact.	An object is interfering with the footrest while the chair is moving, and the chair stops in the middle.	Remove the cause of the emergency stop, and move the chair. When the chair moves properly, the error code will go off.	
C06: Cancelled. Backrest is in contact.	An object is interfering with the backrest while the chair is moving, and the chair stops in the middle.		
C07: Cancelled. Rear link cover is in contact.	An object is interfering with the rear link cover while the chair is moving, and the chair stops in the middle.		
C08: Cancelled. Utility box is in contact.	An object is interfering with the top surface of the junction box while the chair is moving, and the chair stops in the middle.	Remove the cause of the emergency stop, fix the lid of the junction box back in place, and move the chair.	
C09: Cancelled. FC is in contact.	The pedal is stepped on while the chair is moving, and the chair stops in the middle.	Release the pedal of the foot controller, and move the chair. When the chair moves properly, the error code will go off.	
C10: Wait. Chair is warming up.	When the temperature is low, the chair warming-up function is activated.	Wait until the error code goes off (or warming up is completed)	
C12: First priority (Handpiece)	The priority function is activated.	Return all the handpieces to the instrument holder. If the error code does not go off, contact your local authorized Belmont dealer.	
C13: Return handpiece to holder.	A handpiece is not placed in the instrument holder when the power is turned on.	Check that all the handpieces are placed in the instrument holder. If the error code does not go off with all the handpieces in place, contact your local authorized Belmont dealer.	
C14: LP position	When the chair is to be moved from the last position to the gargle position, the chair is already at the gargle position	Move the chair using a switch other than the last position switch.	

10 Accessories and Consumables

10-1 Accessories

Instructions for Use (this document)
Installation Instructions
Declaration of Conformity
Cable (only for the wireless foot controller)
Nozzle cleaning tool (BT14 syringe)



Clip for flushing (BT14 syringe))



10-2 Consumables

Consumables are parts that will normally wear or deteriorate, change their appearance, or become damaged after use. Please note that repair or replacement of consumables are not covered by the warranty and will be charged for.

(* Degree of wear, deterioration or damage and timing for replacement depends on the use environment and conditions at the customer's premises.)

Consumables (Parts listed below are out of the guarantee coverage and charged parts.)

[Reference] List of service parts required for the periodic inspection [page 256]



TAKARA COMPANY EUROPE GmbH

Industriestrasse 21, 61381 Friedrichsdorf, Germany





Albo-Healthcare GmbH

Alte Steinhauserstrasse 19 CH-6330 Cham



TAKARA BELMONT CORPORATION

2-1-1, Higashishinsaibashi, Chuo-ku, Osaka, 542-0083, Japan

TEL: +81-6-6213-5945 FAX: +81-6-6212-3680